


# Stabilitätstest

## Chromatogram Information

User Name user  
 Date Modified 25.03.2021 12:04:18  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 25.03.2021 11:44:29  
 Volume 10,00 [µL]  
 Sample # 4  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

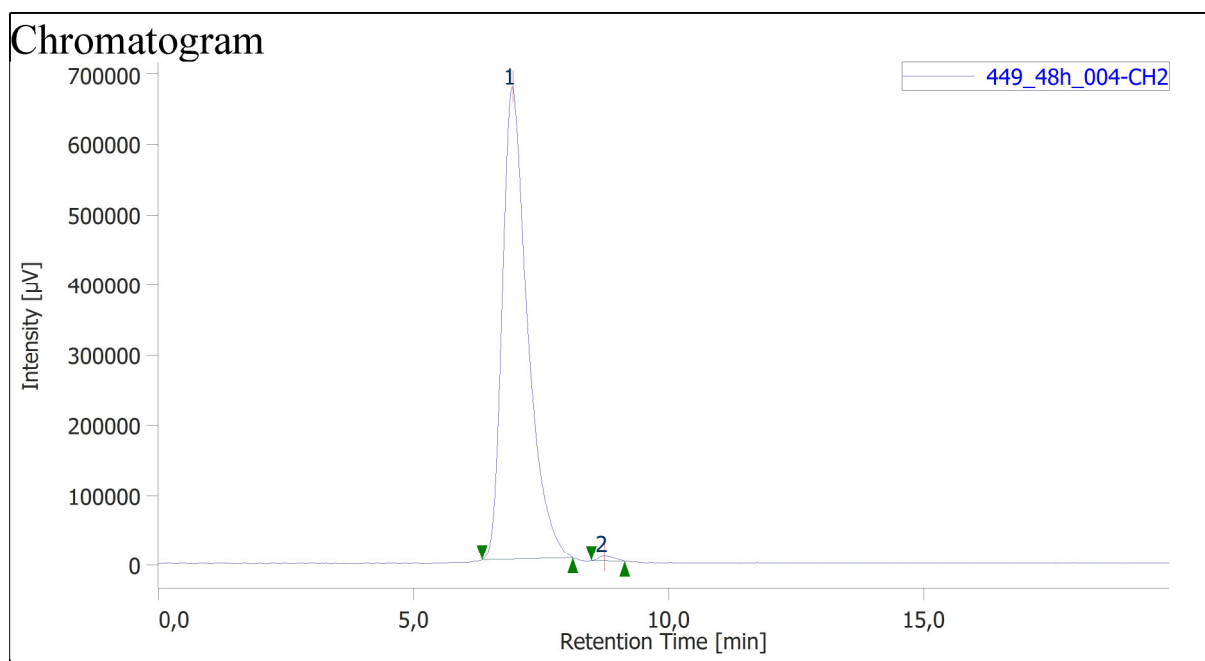

## Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	23089505	673116	99,379	99,007	1030	2,471	1,491
2	Unknown	2	8,742	144317	6750	0,621	0,993	3448	N/A	1,255

