


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 08.09.2021 14:08:38
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 08.09.2021 13:48:49
 Volume 10,00 [μL]
 Sample # 6
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

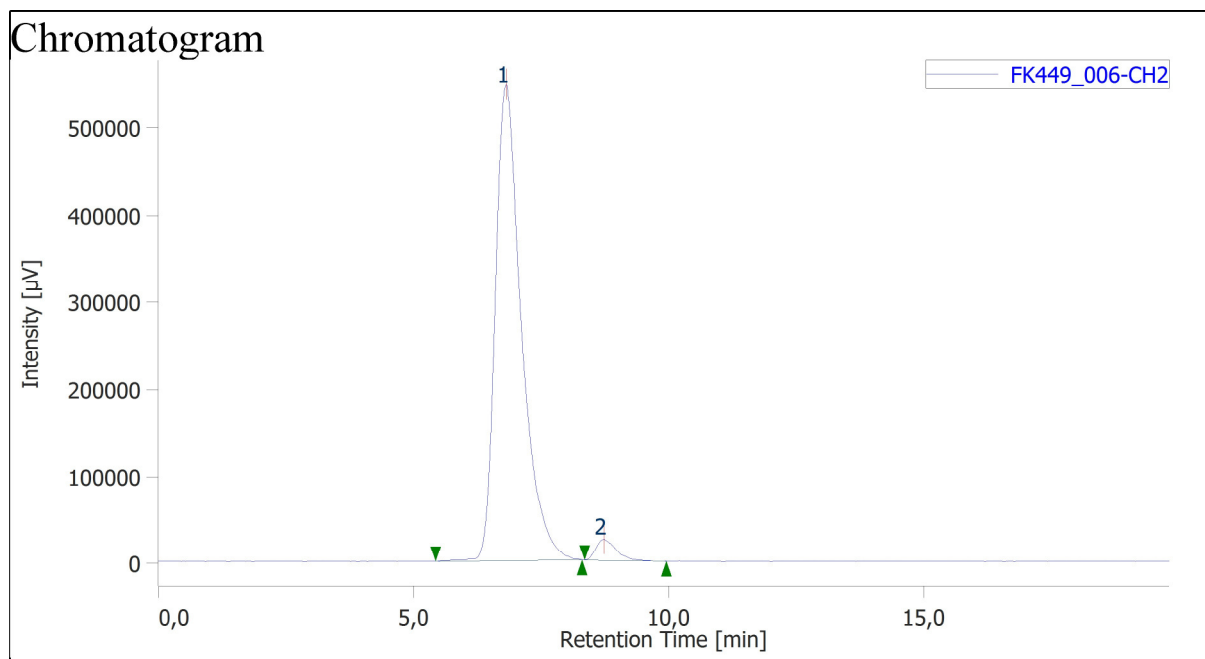

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,817	19412643	546304	96,619	95,638	952	2,390	1,468
2	Unknown	2	8,725	679238	24917	3,381	4,362	2369	N/A	1,530

