


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 06.09.2021 15:15:28
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 06.09.2021 14:33:57
 Volume 10,00 [μL]
 Sample # 8
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

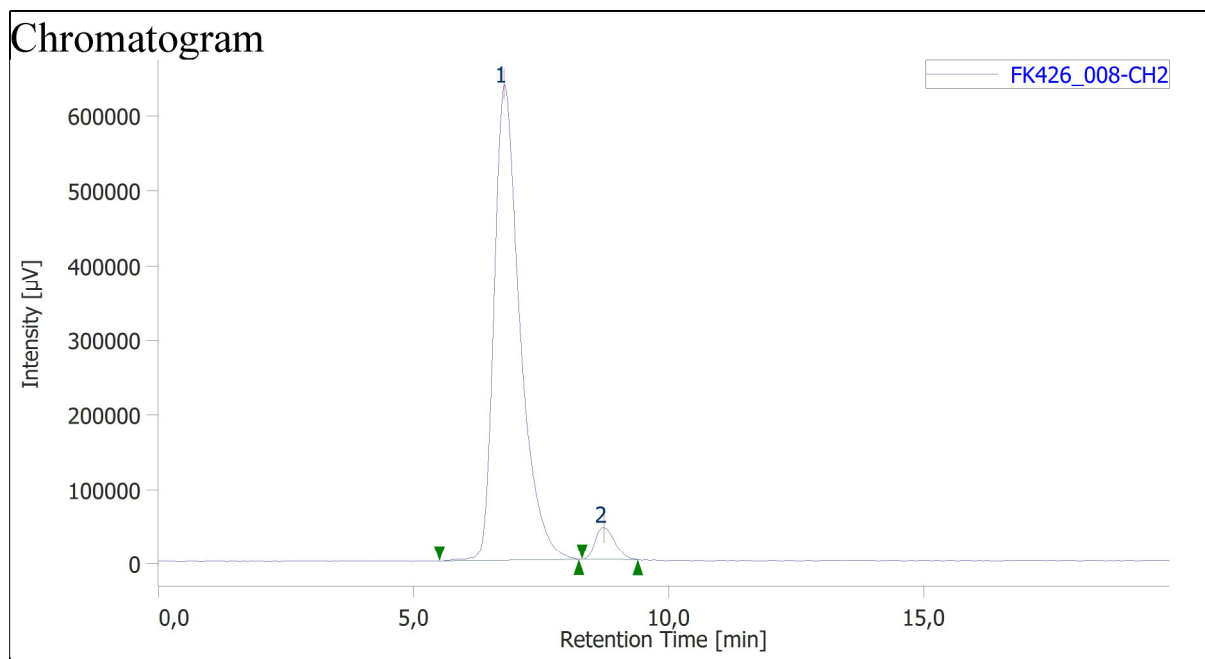

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,775	22430588	636671	95,027	93,606	954	2,465	1,534
2	Unknown	2	8,733	1173912	43490	4,973	6,394	2382	N/A	1,218

