


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 08.09.2021 12:30:55
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 08.09.2021 12:11:06
 Volume 10,00 [µL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

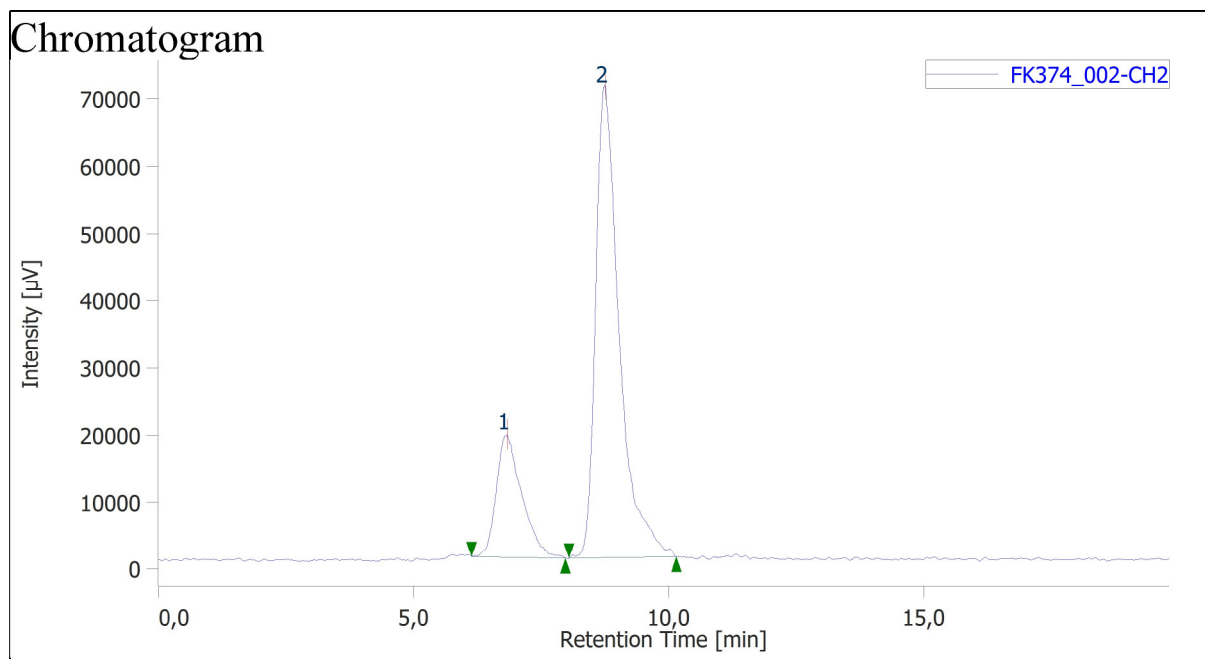

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,833	640014	18354	22,024	20,663	950	2,313	1,335
2	Unknown	2	8,750	2266026	70473	77,976	79,337	2041	N/A	1,716

