


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 07.09.2021 12:25:03
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 07.09.2021 11:51:32
 Volume 10,00 [μL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

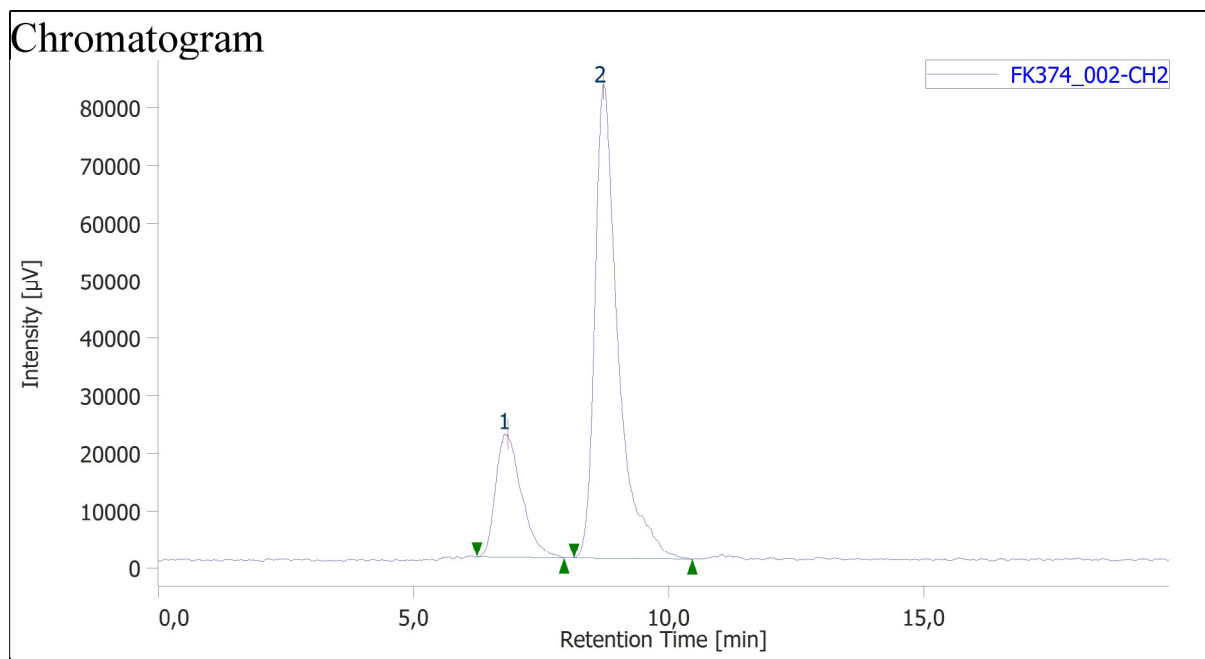

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,842	767147	21561	22,794	20,742	857	2,245	1,378
2	Unknown	2	8,717	2598406	82386	77,206	79,258	2217	N/A	1,774

