


## Stabilitätstest

### Chromatogram Information

User Name user  
Date Modified 30.03.2021 08:54:14  
Description  
HPLC System Name Jasco-HPLC-1  
Injection Date 30.03.2021 08:34:25  
Volume 10,00 [μL]  
Sample # 1  
Project Name Lu-PDL1  
Acquisition Time 19,8 [min]  
Acquisition Sequence  
Control Method PBS\_iso\_20min  
Peak ID Table  
Calibration Method  
Additional Information  
Column Info

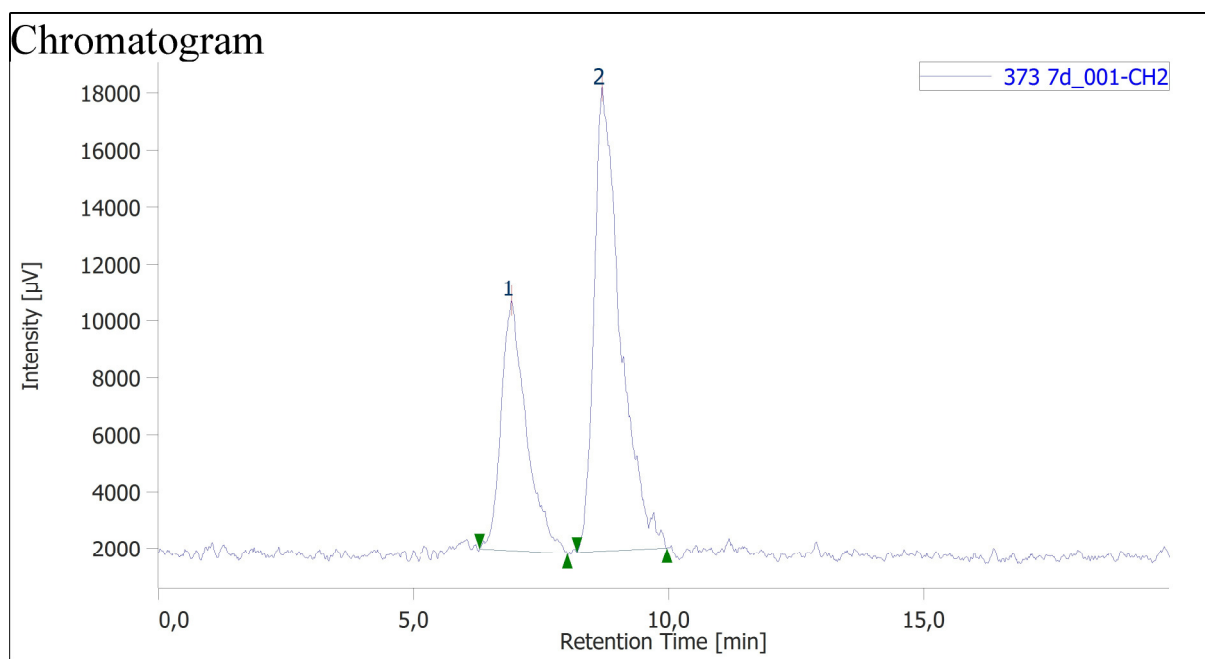

### Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,917	302285	8780	34,152	34,988	1042	2,136	1,517
2	Unknown	2	8,692	582840	16314	65,848	65,012	1846	N/A	1,903

