


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 26.03.2021 13:42:34
Description
HPLC System Name Jasco-HPLC-1
Injection Date 26.03.2021 10:40:59
Volume 10,00 [µL]
Sample # 3
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

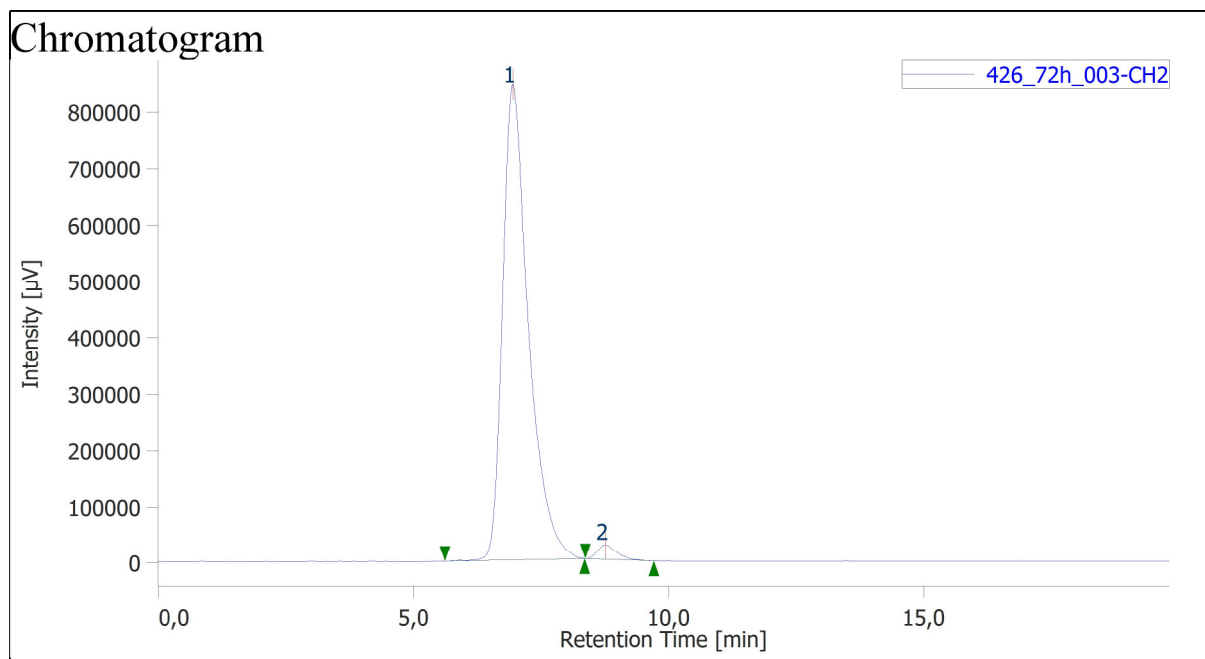

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	29665337	843343	97,777	96,949	1007	2,380	1,524
2	Unknown	2	8,758	674438	26544	2,223	3,051	2852	N/A	1,411

