


# Stabilitätstest

## Chromatogram Information

User Name user  
 Date Modified 09.09.2021 11:46:00  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 09.09.2021 11:26:11  
 Volume 10,00 [μL]  
 Sample # 1  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

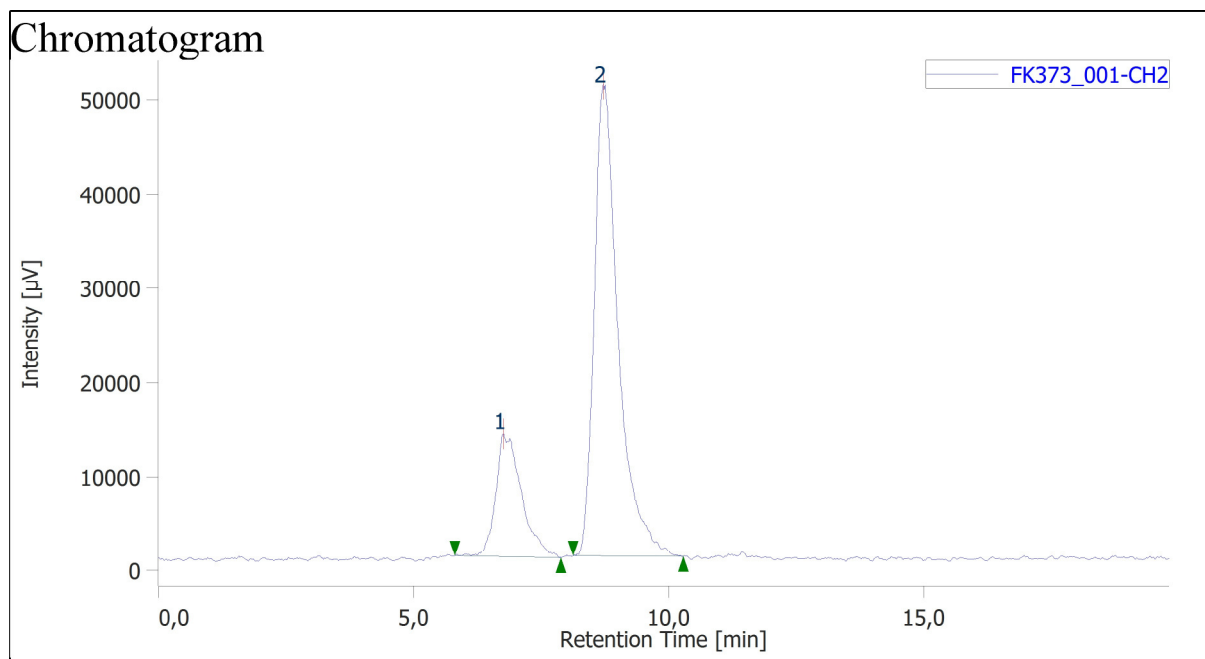

## Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,758	462123	13079	22,064	20,712	912	2,353	1,619
2	Unknown	2	8,717	1632337	50068	77,936	79,288	2031	N/A	1,666

