


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 07.09.2021 12:25:02
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 07.09.2021 11:30:44
 Volume 10,00 [μL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

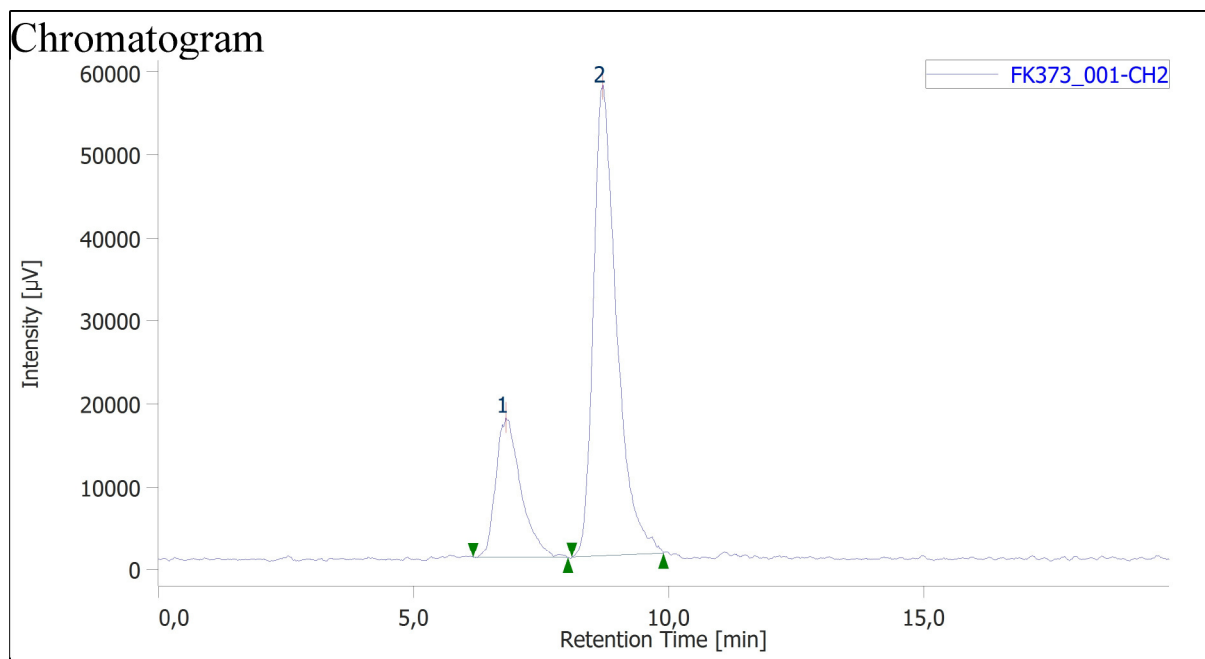

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,808	577982	16882	24,335	22,926	1017	2,340	1,492
2	Unknown	2	8,708	1797122	56757	75,665	77,074	2024	N/A	1,511

