


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 09.09.2021 12:29:14
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 09.09.2021 12:09:25
 Volume 10,00 [μL]
 Sample # 3
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

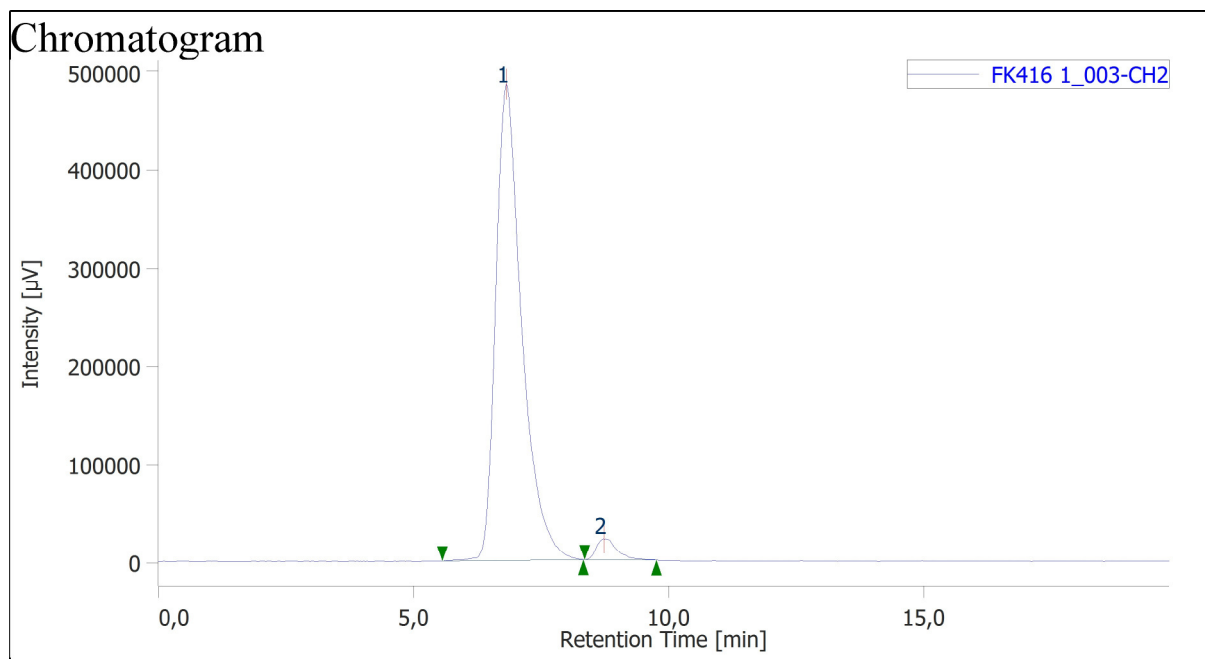

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,817	17168849	483843	96,514	95,623	951	2,404	1,512
2	Unknown	2	8,725	620199	22148	3,486	4,377	2432	N/A	1,737

