


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 26.03.2021 09:44:37
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 26.03.2021 09:24:47
 Volume 10,00 [µL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

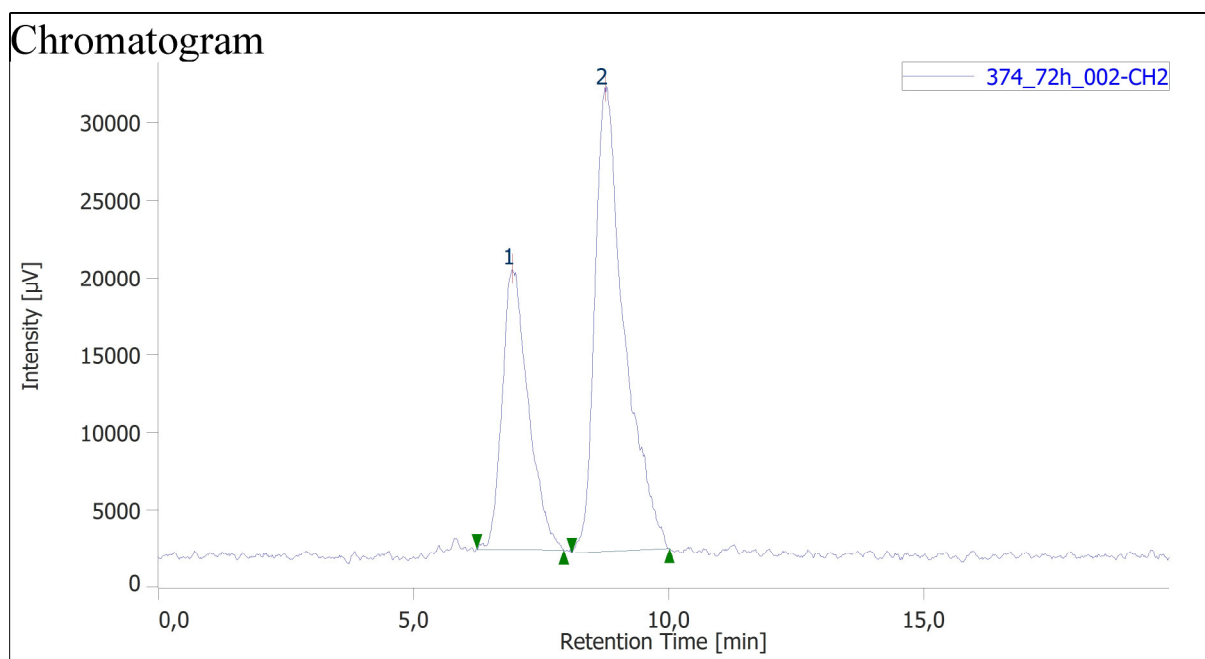

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,933	646136	18125	35,029	37,674	925	1,954	1,424
2	Unknown	2	8,750	1198424	29985	64,971	62,326	1349	N/A	1,673

