


## Stabilitätstest

### Chromatogram Information

User Name user  
 Date Modified 09.09.2021 12:49:40  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 09.09.2021 12:29:50  
 Volume 10,00 [μL]  
 Sample # 4  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

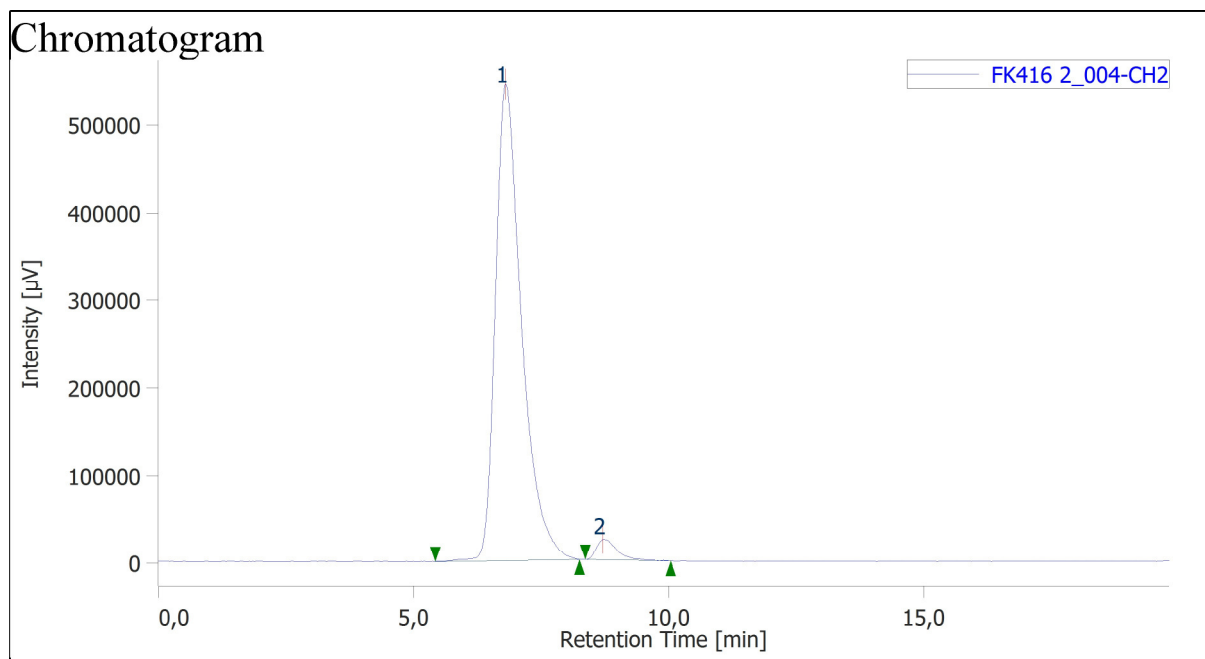

### Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,800	19344174	542661	96,665	95,722	928	2,396	1,550
2	Unknown	2	8,708	667387	24255	3,335	4,278	2445	N/A	1,893

