


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 06.09.2021 13:23:51
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 06.09.2021 11:40:07
 Volume 20,00 [µL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

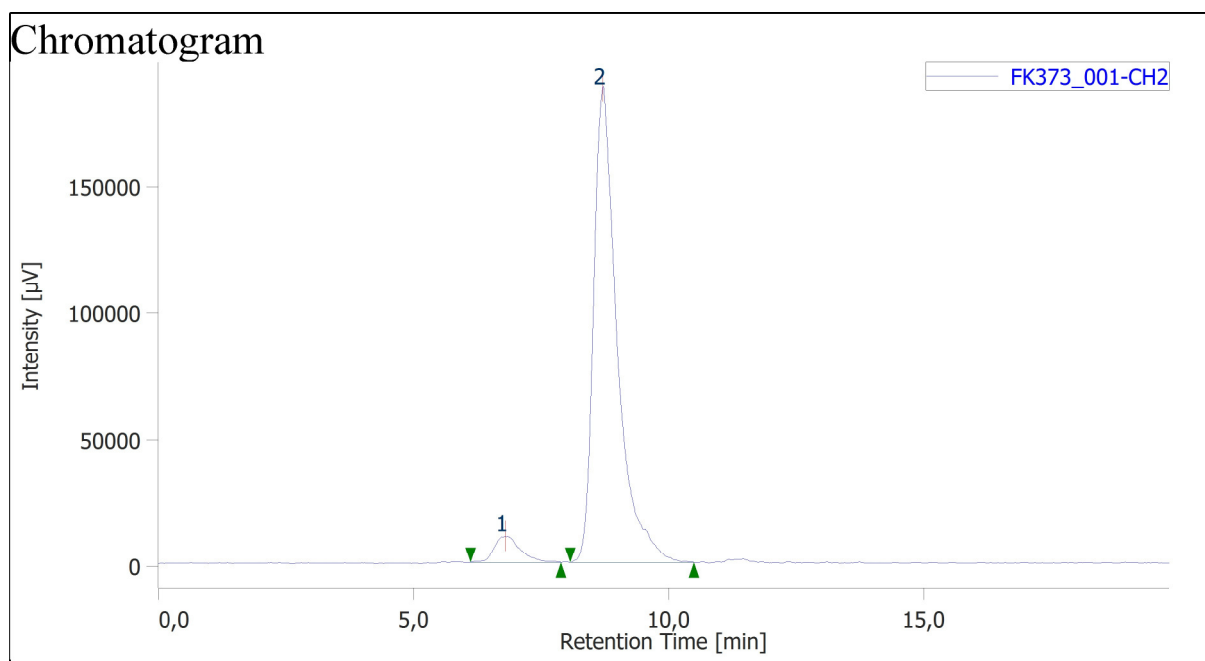

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,792	376616	10668	5,884	5,374	917	2,307	1,352
2	Unknown	2	8,708	6024159	187858	94,116	94,626	2052	N/A	1,682

