


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 31.08.2021 14:33:07
Description
HPLC System Name Jasco-HPLC-1
Injection Date 31.08.2021 13:28:35
Volume 20,00 [μL]
Sample # 1
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

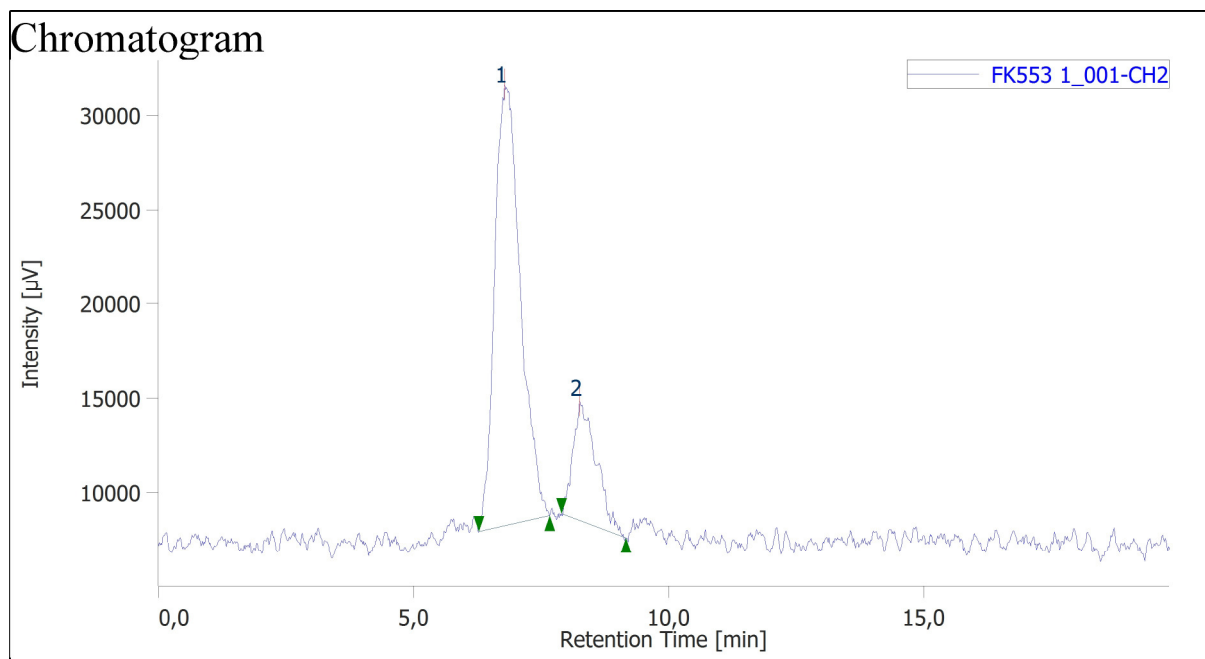

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,783	817177	23375	80,299	78,723	889	1,562	1,337
2	Unknown	2	8,250	200487	6318	19,701	21,277	1149	N/A	1,757

