


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 24.03.2021 12:28:49
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 23.03.2021 14:38:36
 Volume 10,00 [µL]
 Sample # 5
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

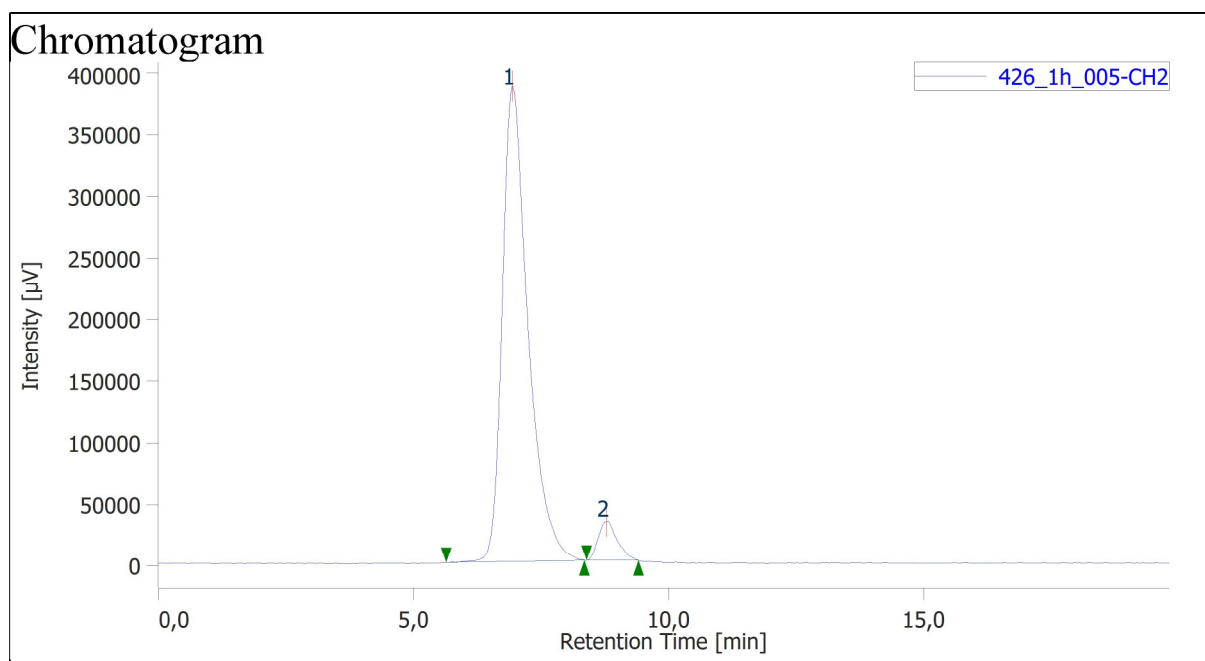

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,933	13528785	385359	94,173	92,314	1013	2,383	1,500
2	Unknown	2	8,775	837047	32085	5,827	7,686	2673	N/A	1,343

