


## Stabilitätstest

### Chromatogram Information

User Name user  
 Date Modified 07.09.2021 14:37:02  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 07.09.2021 13:31:50  
 Volume 10,00 [μL]  
 Sample # 6  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

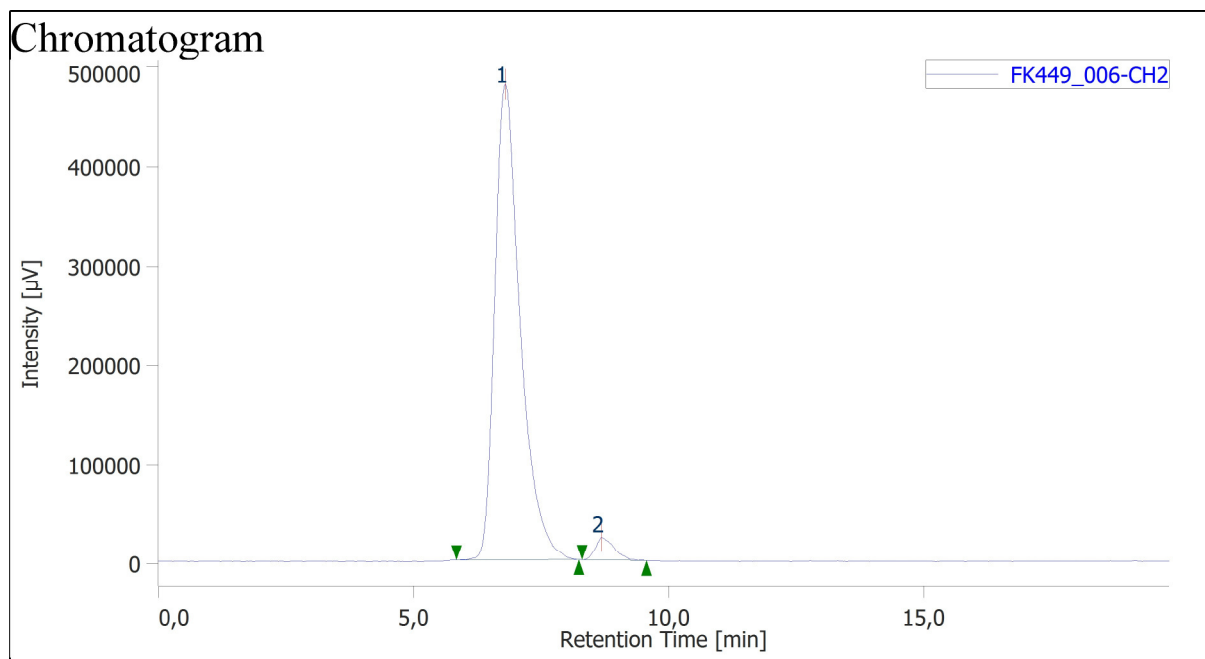

### Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,792	16603350	478340	96,551	95,251	970	2,469	1,502
2	Unknown	2	8,675	593072	23848	3,449	4,749	2785	N/A	1,476

