


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 23.03.2021 11:03:01
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 23.03.2021 10:43:11
 Volume 10,00 [µL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

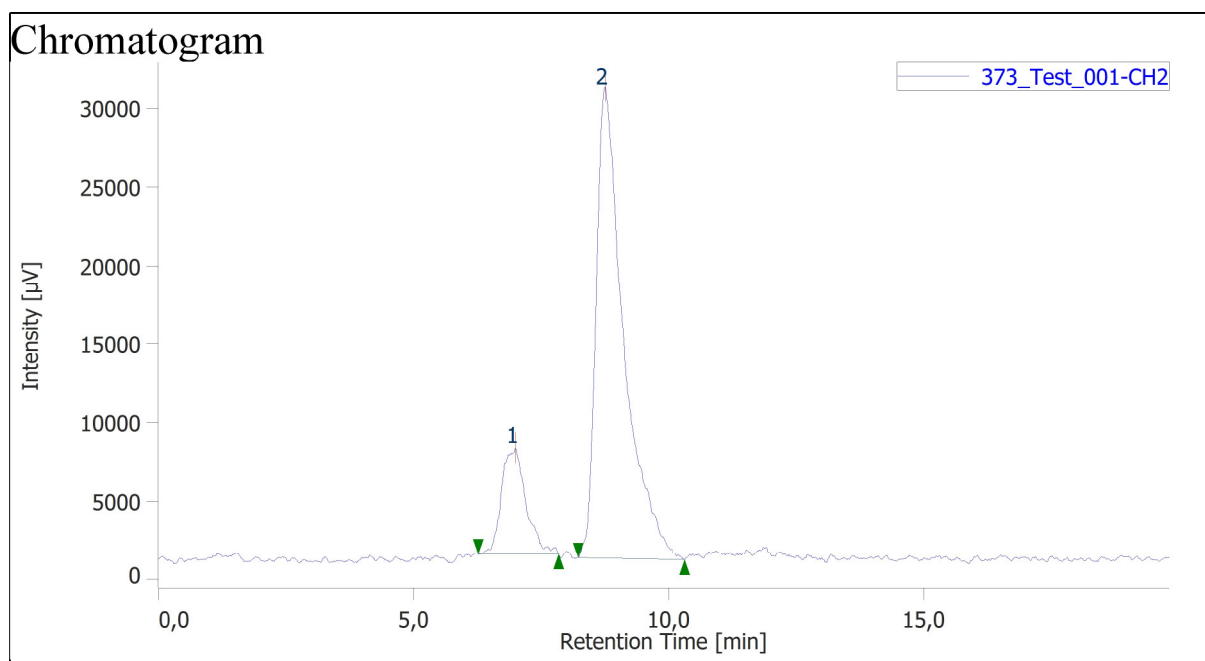

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	7,000	225877	6780	16,701	18,419	1112	2,030	1,243
2	Unknown	2	8,750	1126588	30028	83,299	81,581	1551	N/A	1,991

