


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 09.09.2021 12:06:30
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 09.09.2021 11:46:41
 Volume 10,00 [μL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

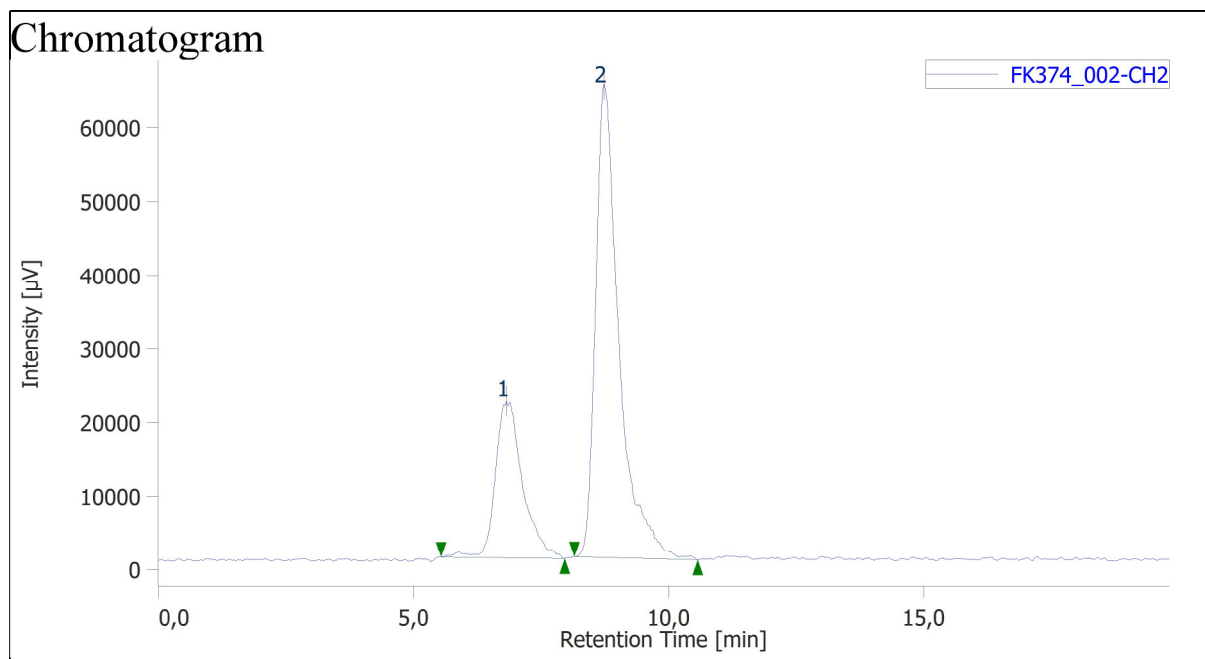

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,817	793284	21270	27,951	24,911	928	2,316	1,511
2	Unknown	2	8,725	2044843	64113	72,049	75,089	2123	N/A	1,870

