


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 06.09.2021 15:15:28
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 06.09.2021 14:13:05
 Volume 10,00 [μL]
 Sample # 7
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

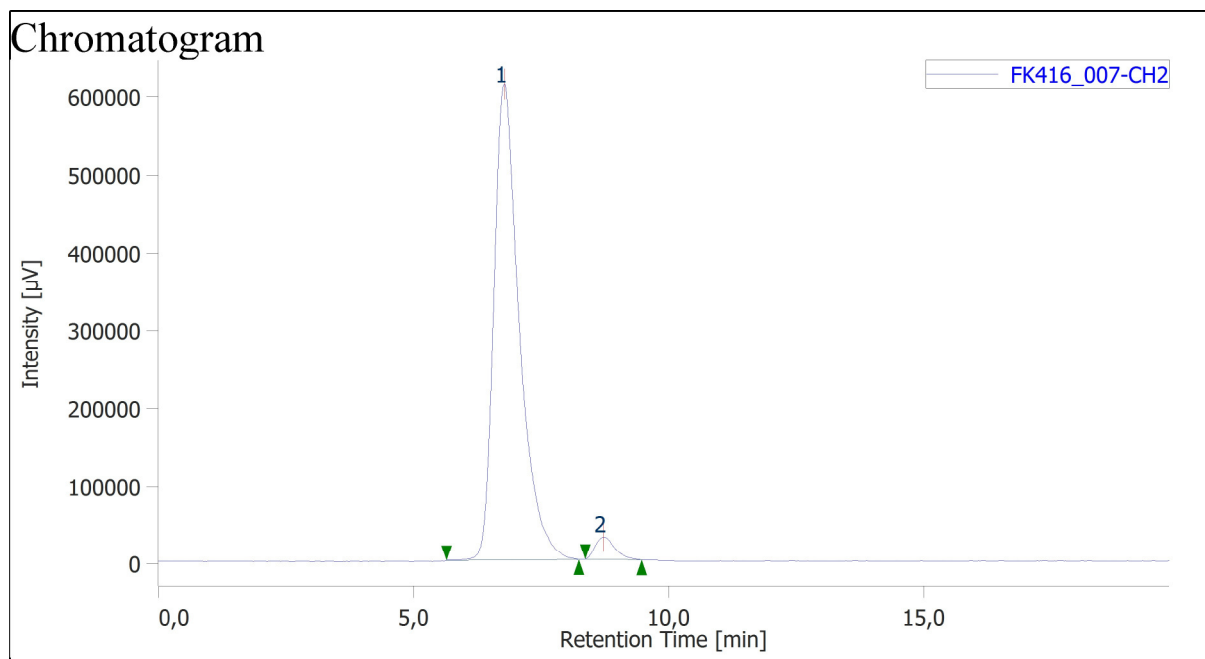

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,783	21208315	610939	96,449	95,416	975	2,476	1,479
2	Unknown	2	8,717	780872	29351	3,551	4,584	2504	N/A	1,407

