


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 01.09.2021 14:30:22
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 01.09.2021 13:16:27
 Volume 20,00 [µL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

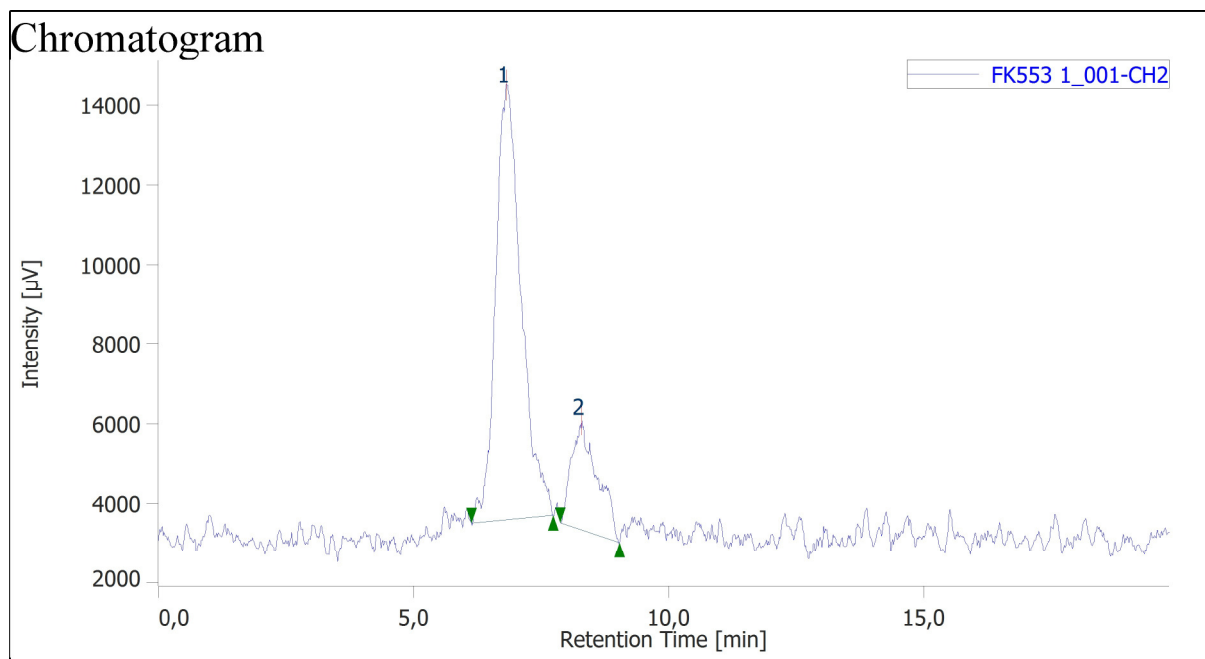

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,825	379583	10894	79,870	79,811	948	1,561	1,187
2	Unknown	2	8,292	95669	2756	20,130	20,189	1104	N/A	1,396

