


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 07.09.2021 13:34:15
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 07.09.2021 13:10:59
 Volume 10,00 [μL]
 Sample # 5
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

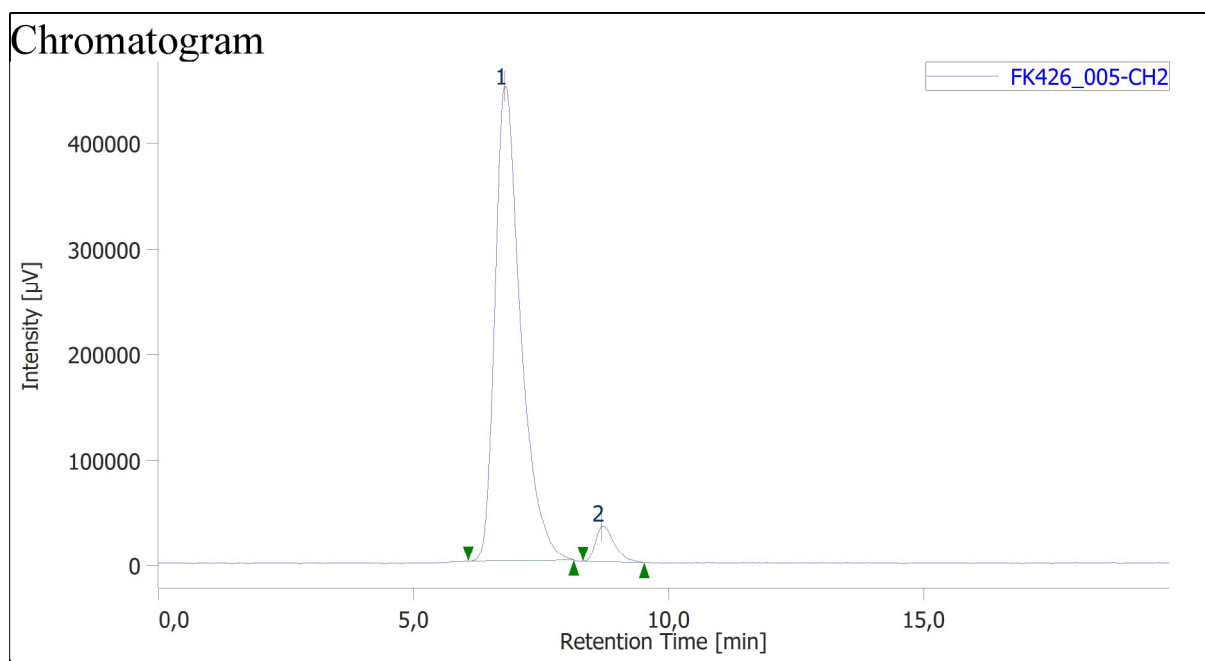

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,783	15702016	448800	94,639	92,895	973	2,482	1,551
2	Unknown	2	8,683	889435	34325	5,361	7,105	2727	N/A	1,633

