


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 06.09.2021 13:23:51
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 06.09.2021 12:47:33
 Volume 20,00 [μL]
 Sample # 3
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

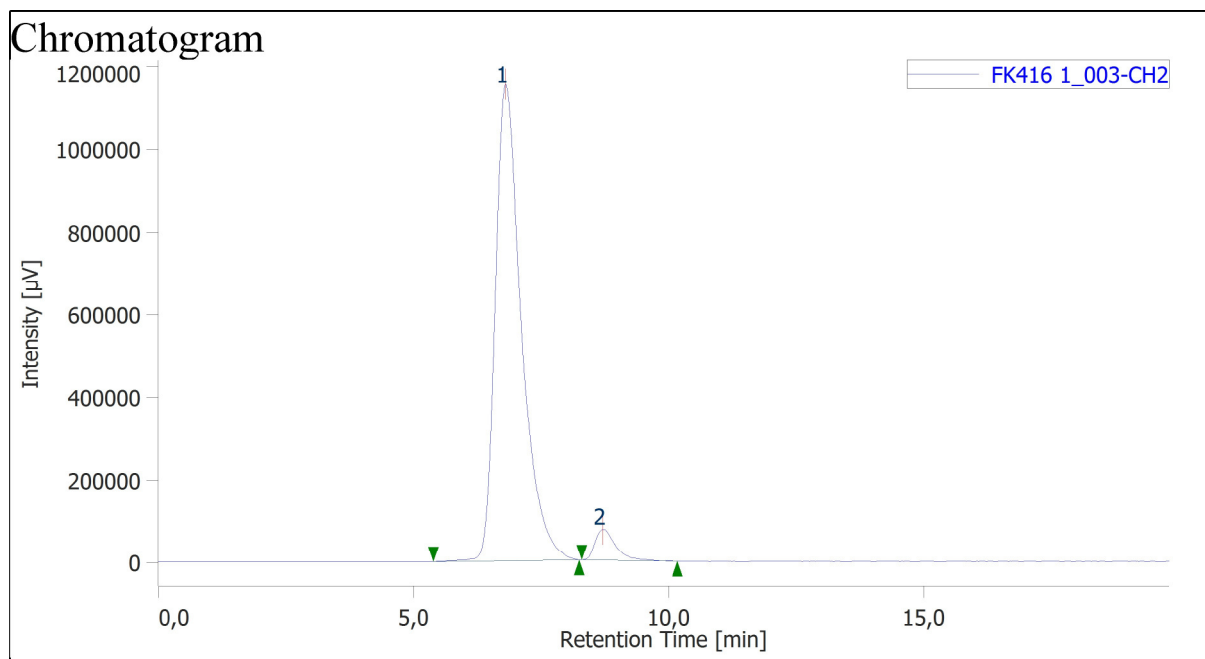

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,800	41012331	1152255	95,030	93,827	943	2,400	1,530
2	Unknown	2	8,708	2144737	75808	4,970	6,173	2414	N/A	1,655

