


## Stabilitätstest

### Chromatogram Information

User Name user  
 Date Modified 06.09.2021 13:23:51  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 06.09.2021 12:26:28  
 Volume 20,00 [µL]  
 Sample # 2  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

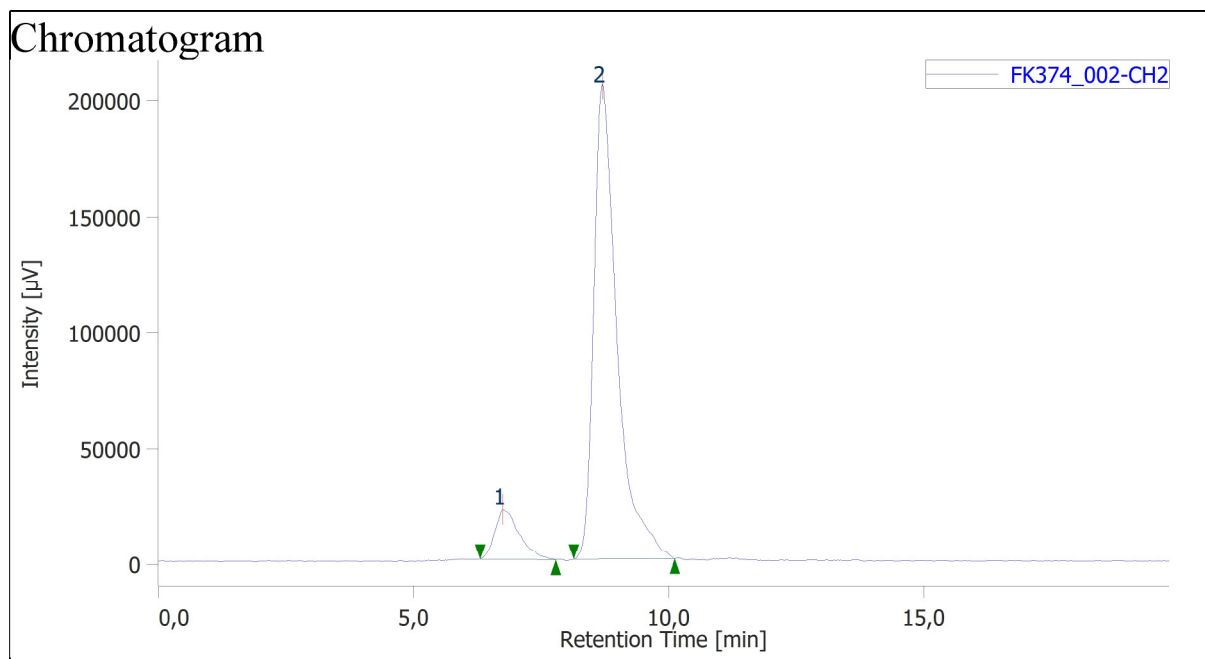

### Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,750	729956	21816	10,127	9,629	986	2,411	1,634
2	Unknown	2	8,700	6478238	204751	89,873	90,371	2085	N/A	1,837

