


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 06.09.2021 15:15:28
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 06.09.2021 14:54:31
 Volume 10,00 [µL]
 Sample # 9
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

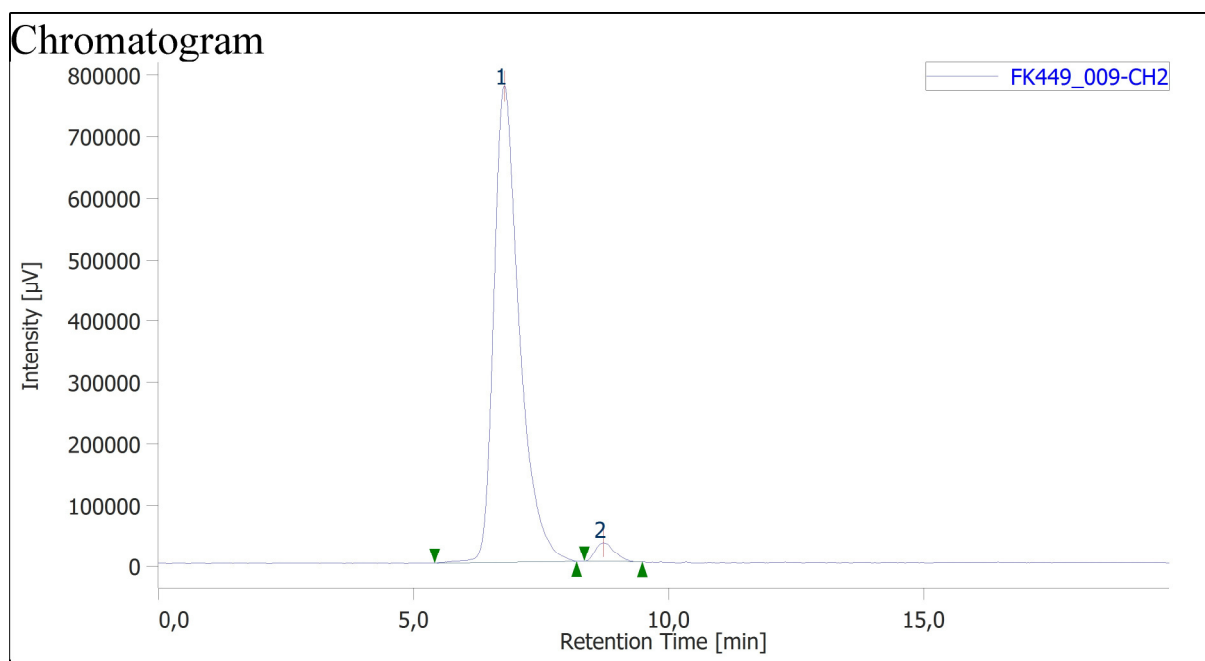

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,783	26969493	774487	97,055	96,087	986	2,451	1,461
2	Unknown	2	8,717	818378	31544	2,945	3,913	2359	N/A	1,326

