


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 25.03.2021 14:52:25
Description
HPLC System Name Jasco-HPLC-1
Injection Date 25.03.2021 10:39:22
Volume 10,00 [µL]
Sample # 3
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

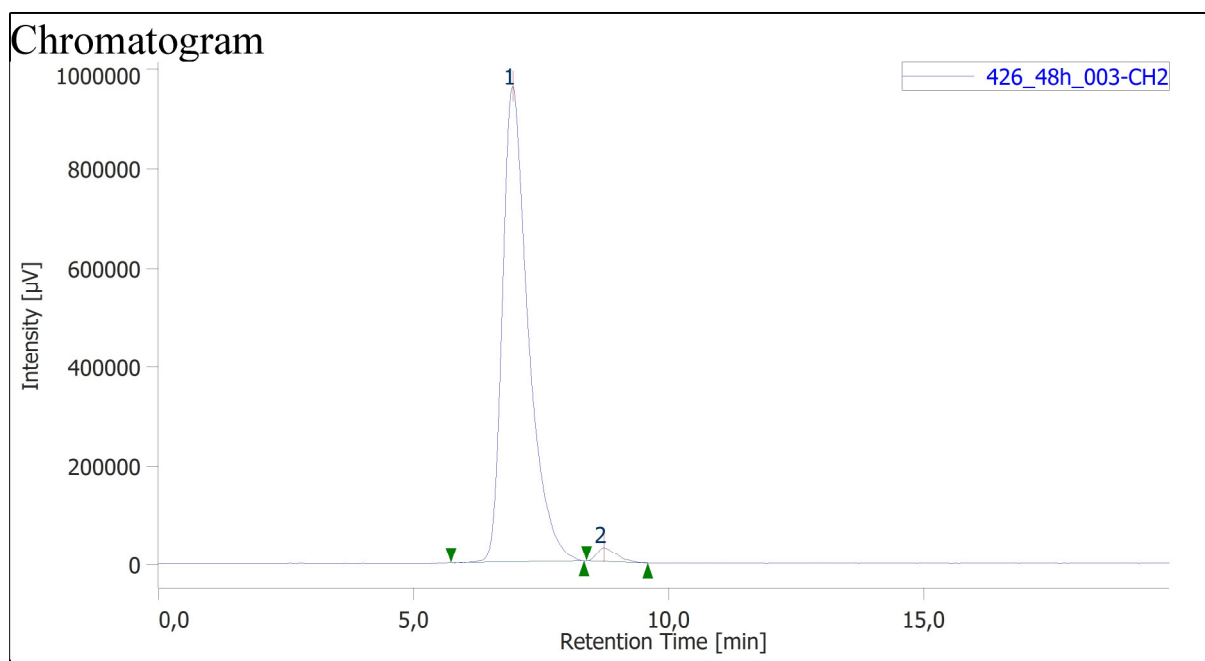

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	33651218	959314	97,819	97,070	1019	2,278	1,521
2	Unknown	2	8,725	750251	28958	2,181	2,930	2488	N/A	1,583

