


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 30.08.2021 16:34:07
Description
HPLC System Name Jasco-HPLC-1
Injection Date 30.08.2021 15:38:58
Volume 10,00 [μL]
Sample # 1
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

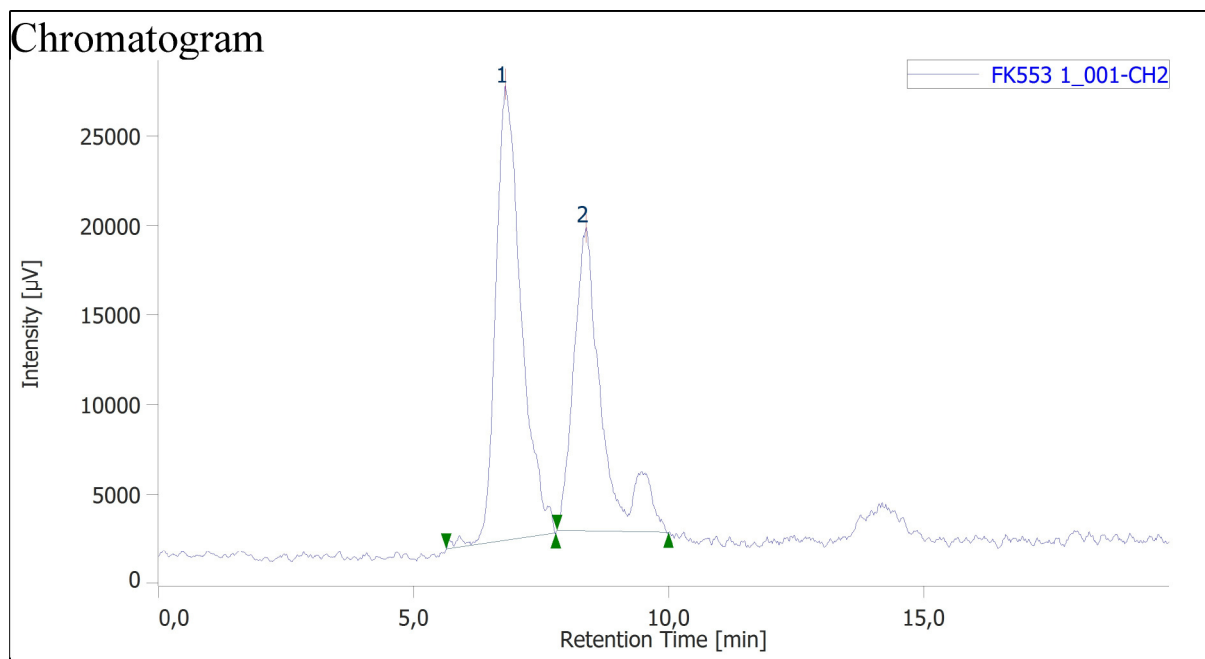

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,792	875335	25401	57,227	59,996	987	1,816	1,618
2	Unknown	2	8,375	654243	16937	42,773	40,004	1438	N/A	1,908

