


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 08.09.2021 13:47:58
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 08.09.2021 13:28:08
 Volume 10,00 [µL]
 Sample # 5
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

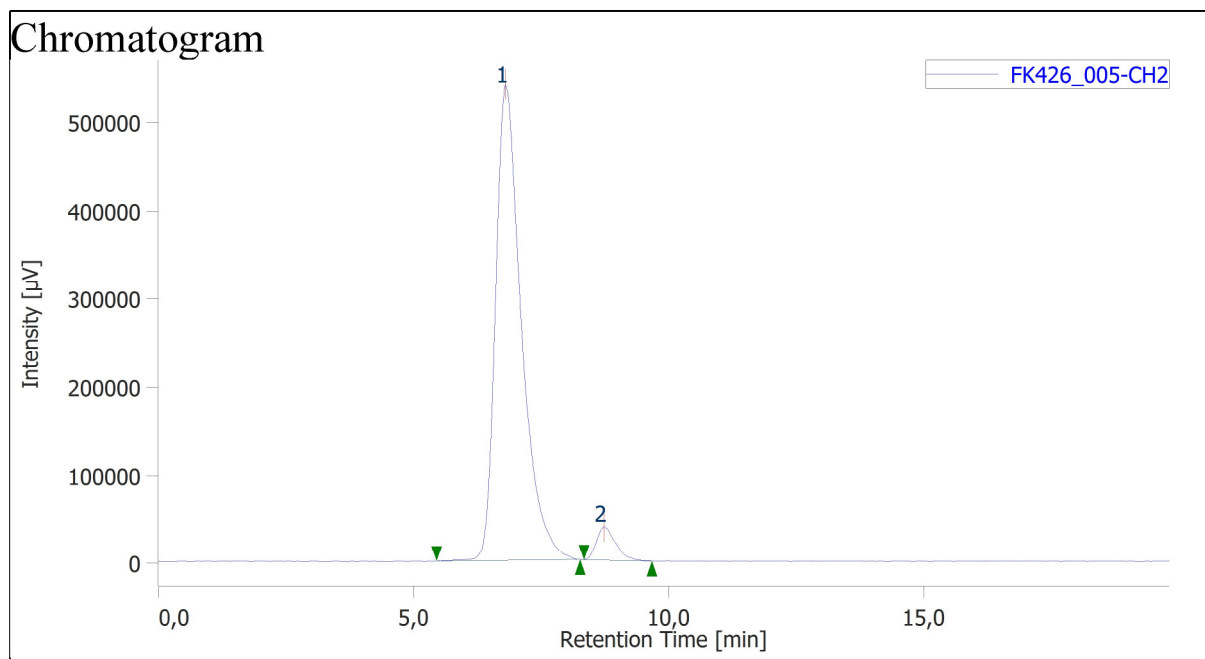

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,800	18975095	539695	94,986	93,320	957	2,469	1,550
2	Unknown	2	8,725	1001660	38635	5,014	6,680	2600	N/A	1,435

