


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 24.03.2021 16:43:04
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 24.03.2021 09:43:56
 Volume 10,00 [µL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

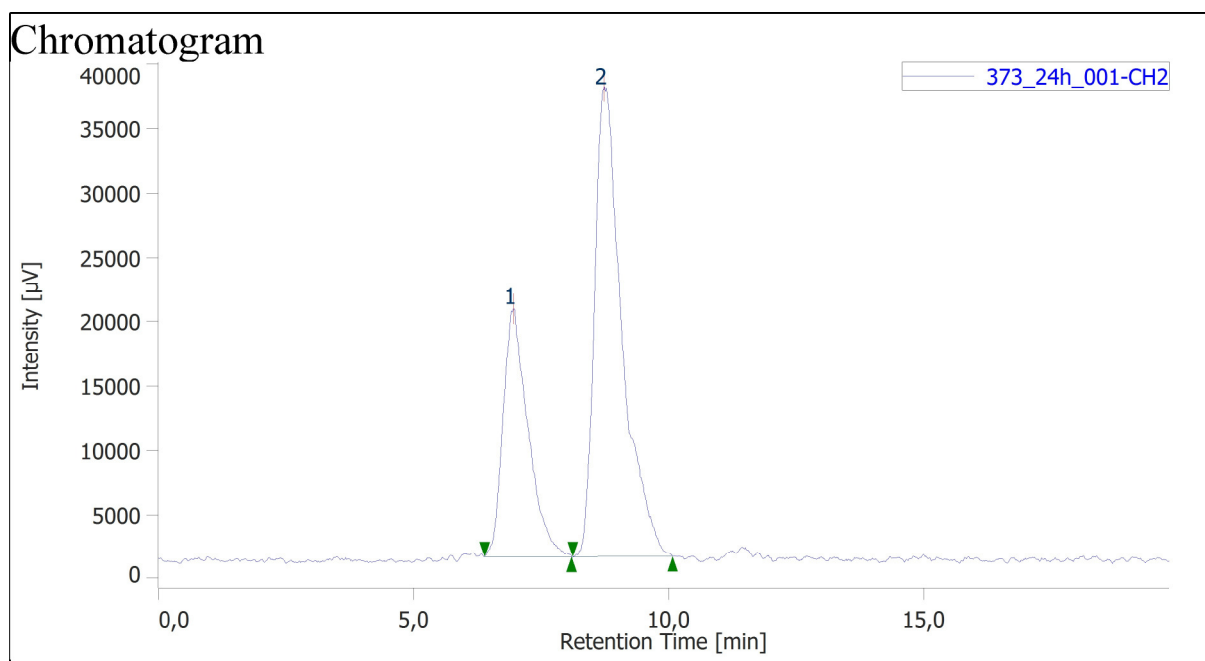

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,958	659011	19259	32,541	34,506	964	1,979	1,434
2	Unknown	2	8,733	1366141	36554	67,459	65,494	1499	N/A	1,735

