


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 24.03.2021 12:28:49
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 23.03.2021 15:58:02
 Volume 10,00 [µL]
 Sample # 7
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

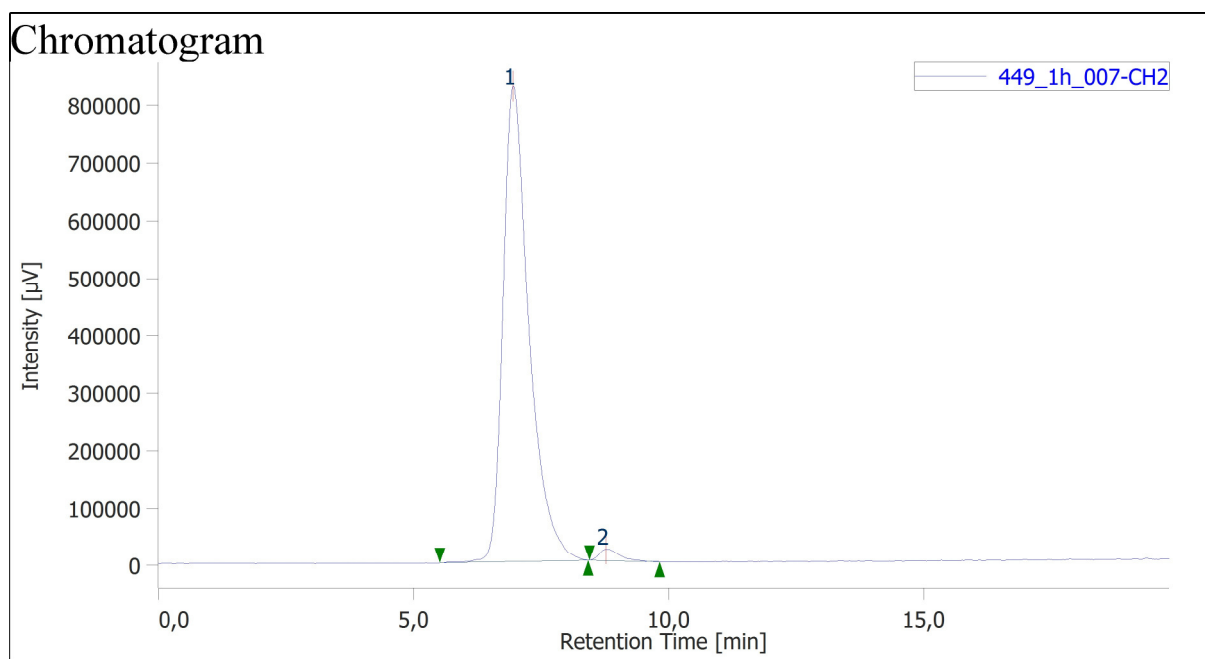

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,950	29366498	825919	98,060	97,590	1004	2,318	1,536
2	Unknown	2	8,767	580989	20394	1,940	2,410	2551	N/A	2,262

