


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 07.09.2021 13:34:15
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 07.09.2021 12:33:34
 Volume 10,00 [μL]
 Sample # 4
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

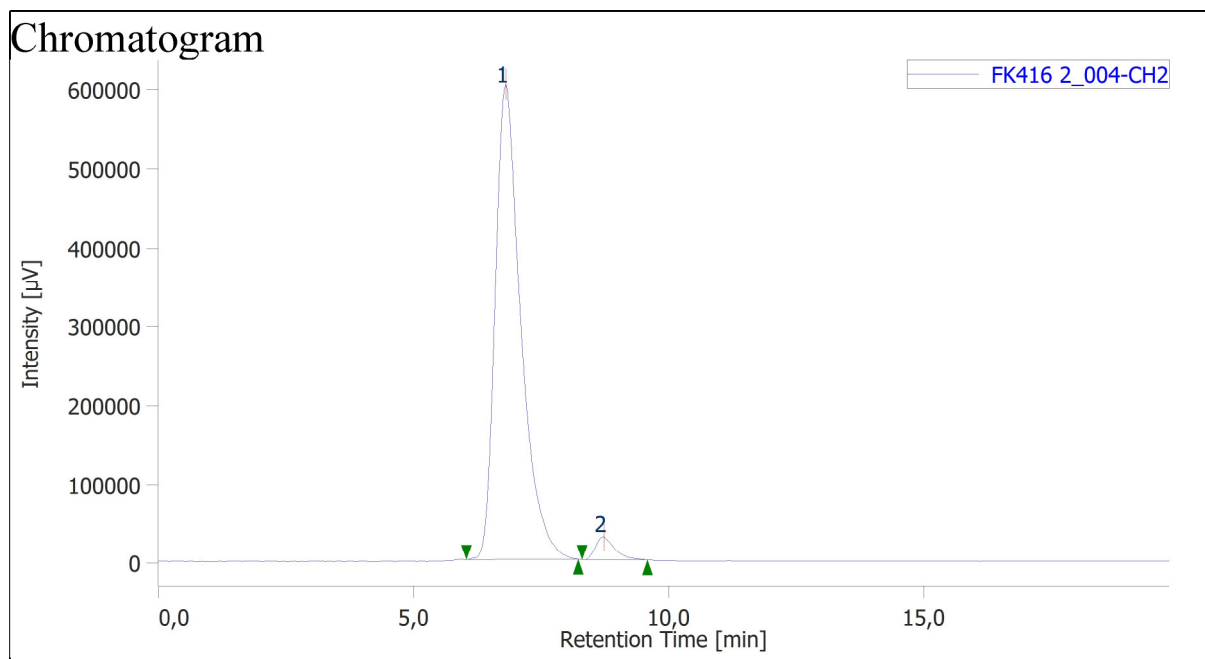

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,808	20981566	602154	96,415	95,222	955	2,497	1,467
2	Unknown	2	8,725	780113	30212	3,585	4,778	2814	N/A	1,485

