


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 01.09.2021 14:30:22
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 01.09.2021 14:09:31
 Volume 20,00 [µL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

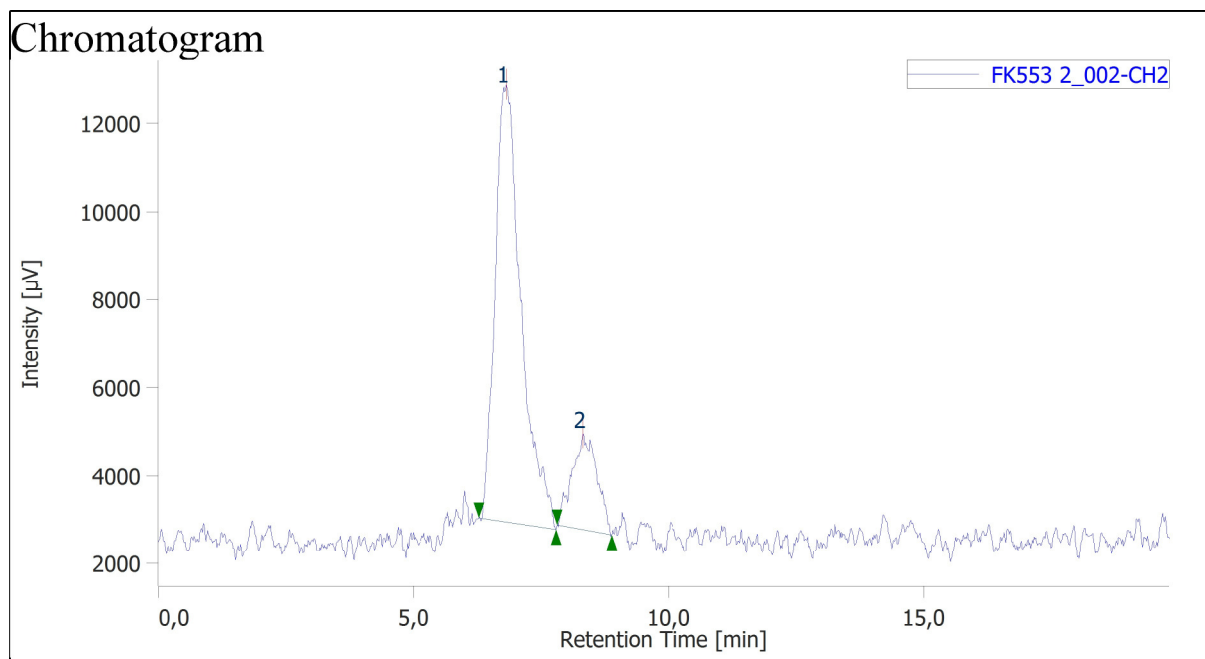

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,817	349795	9925	82,727	81,945	912	1,593	1,526
2	Unknown	2	8,317	73035	2187	17,273	18,055	1141	N/A	1,064

