


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 30.03.2021 09:44:31
Description
HPLC System Name Jasco-HPLC-1
Injection Date 30.03.2021 09:24:43
Volume 10,00 [µL]
Sample # 2
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

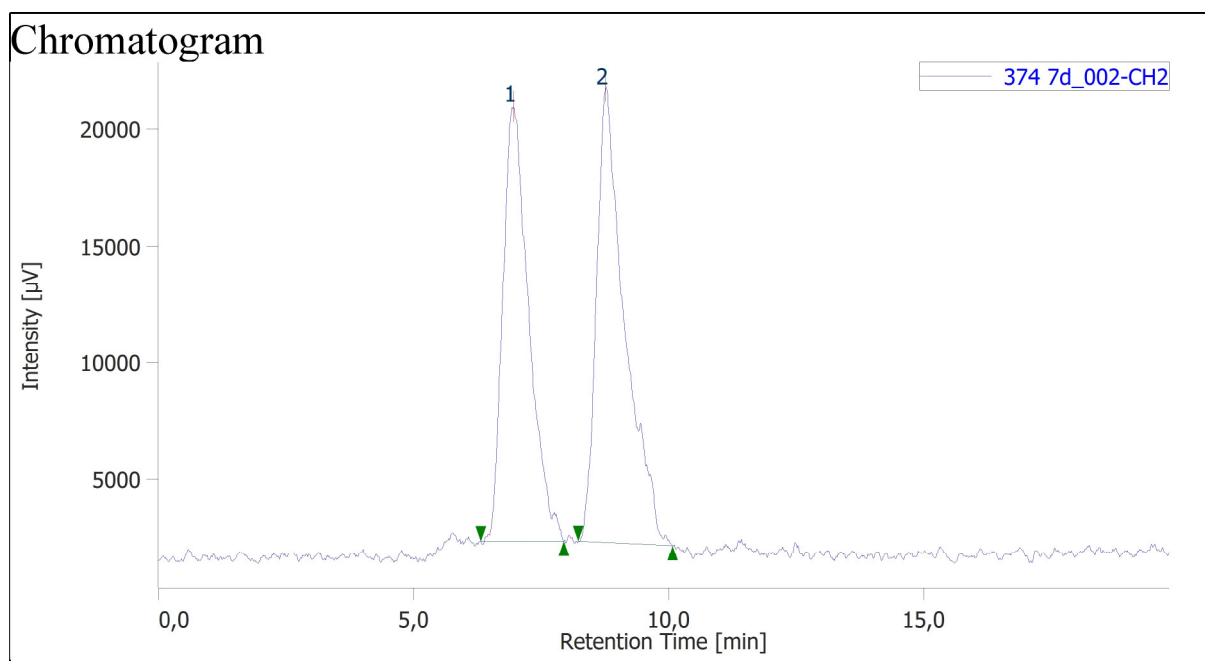

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,958	660597	18615	46,855	48,797	900	1,950	1,516
2	Unknown	2	8,758	749271	19533	53,145	51,203	1440	N/A	1,704

