


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 24.03.2021 10:51:52
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 24.03.2021 10:32:04
 Volume 10,00 [µL]
 Sample # 3
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

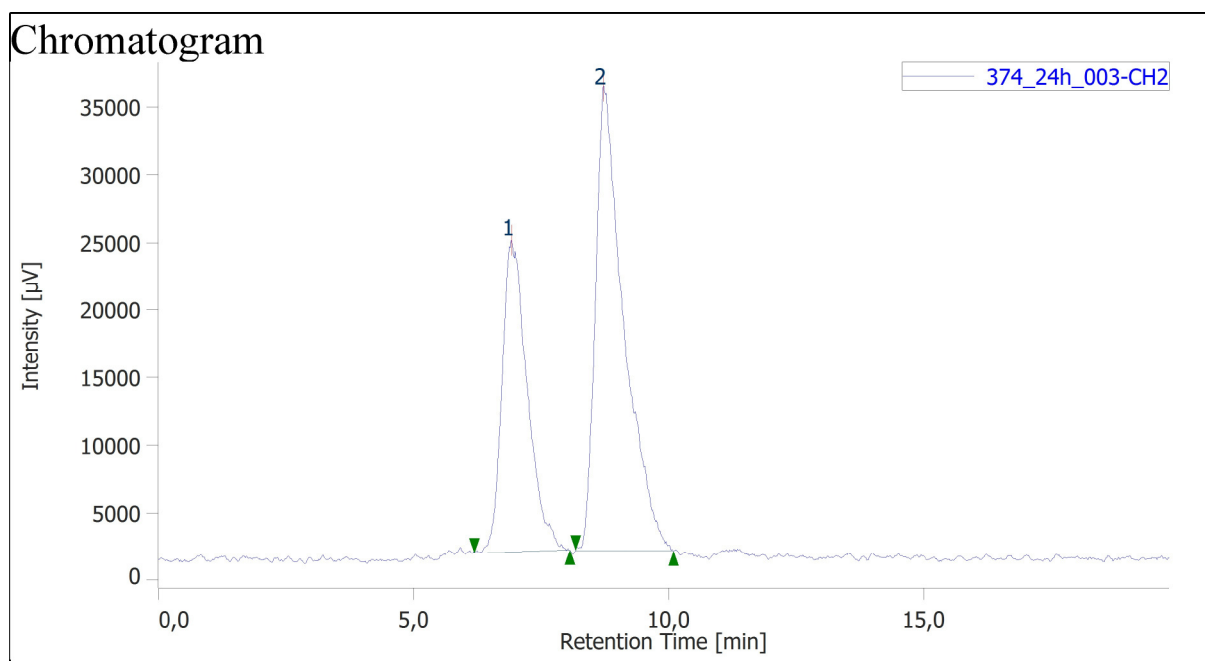

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,917	794296	23075	37,535	40,218	971	1,968	1,486
2	Unknown	2	8,717	1321824	34300	62,465	59,782	1357	N/A	1,987

