


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 09.09.2021 13:45:59
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 09.09.2021 13:26:10
 Volume 10,00 [μL]
 Sample # 5
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

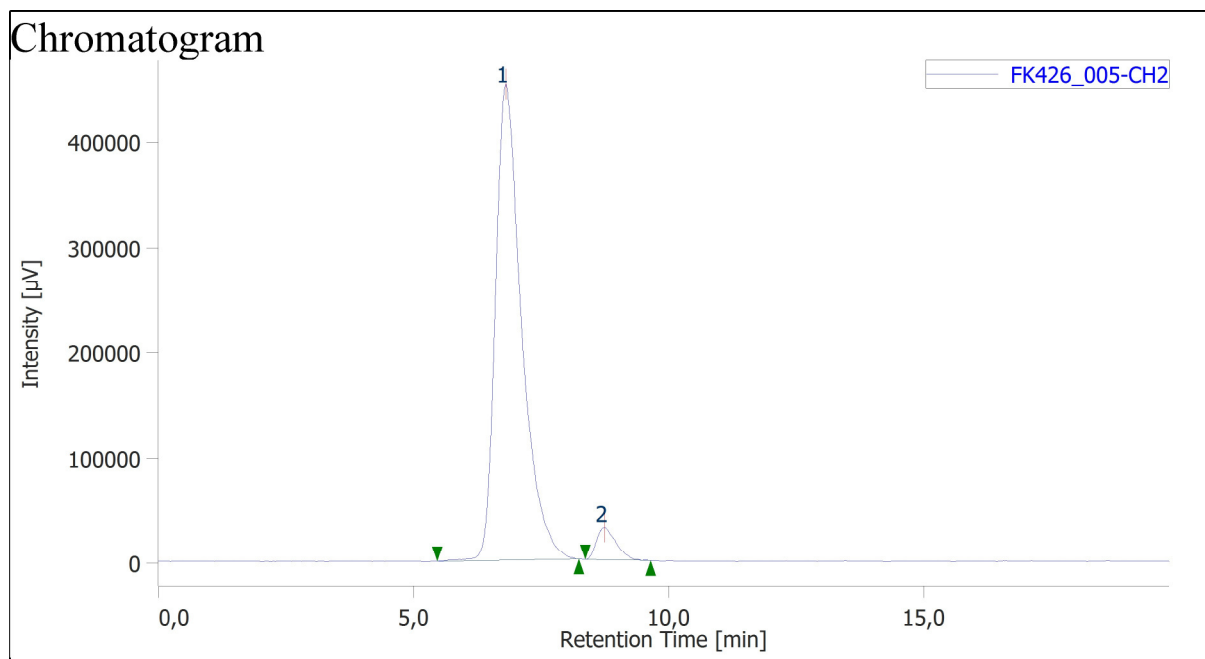

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,808	16063132	451376	95,076	93,439	941	2,435	1,524
2	Unknown	2	8,742	831925	31694	4,924	6,561	2463	N/A	1,368

