


## Stabilitätstest

### Chromatogram Information

User Name user  
Date Modified 26.03.2021 13:42:34  
Description  
HPLC System Name Jasco-HPLC-1  
Injection Date 26.03.2021 11:57:52  
Volume 8,00 [µL]  
Sample # 6  
Project Name Lu-PDL1  
Acquisition Time 19,8 [min]  
Acquisition Sequence  
Control Method PBS\_iso\_20min  
Peak ID Table  
Calibration Method  
Additional Information  
Column Info

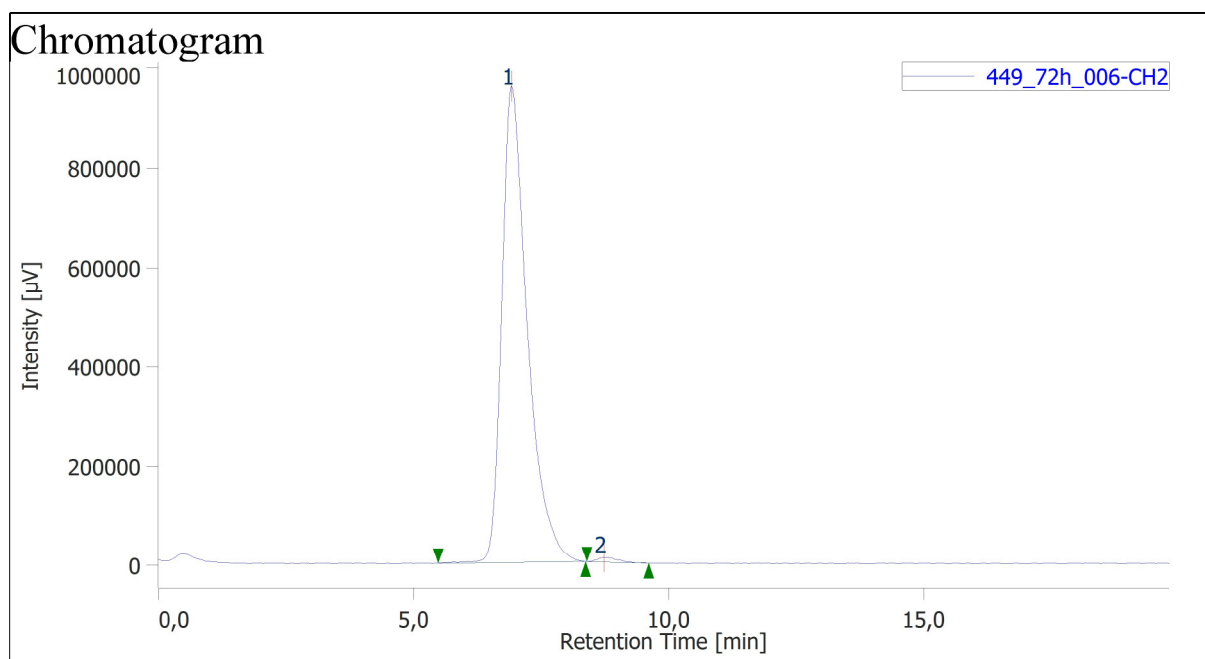

### Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,917	33332892	957133	99,204	98,979	1018	2,248	1,567
2	Unknown	2	8,725	267423	9874	0,796	1,021	2187	N/A	2,008

