


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 31.08.2021 14:33:07
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 31.08.2021 13:58:55
 Volume 20,00 [μL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

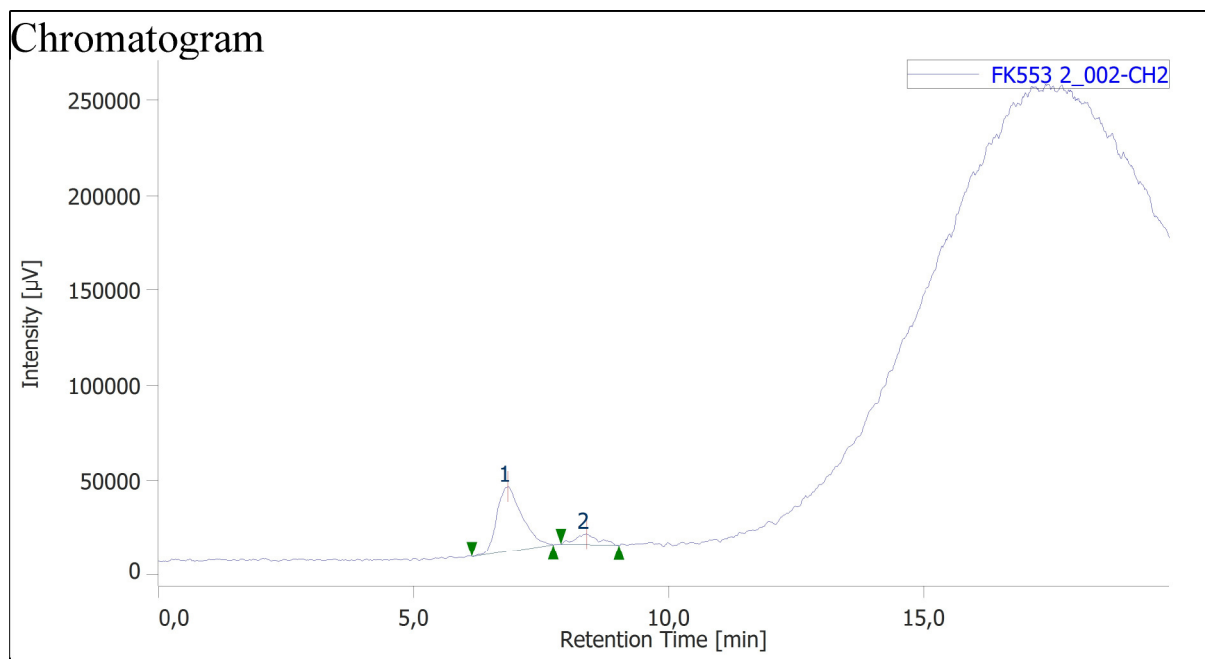

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,850	1168138	34182	86,534	85,516	956	1,950	1,361
2	Unknown	2	8,383	181779	5790	13,466	14,484	2355	N/A	1,084

