


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 24.03.2021 11:34:16
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 24.03.2021 11:14:28
 Volume 10,00 [µL]
 Sample # 5
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

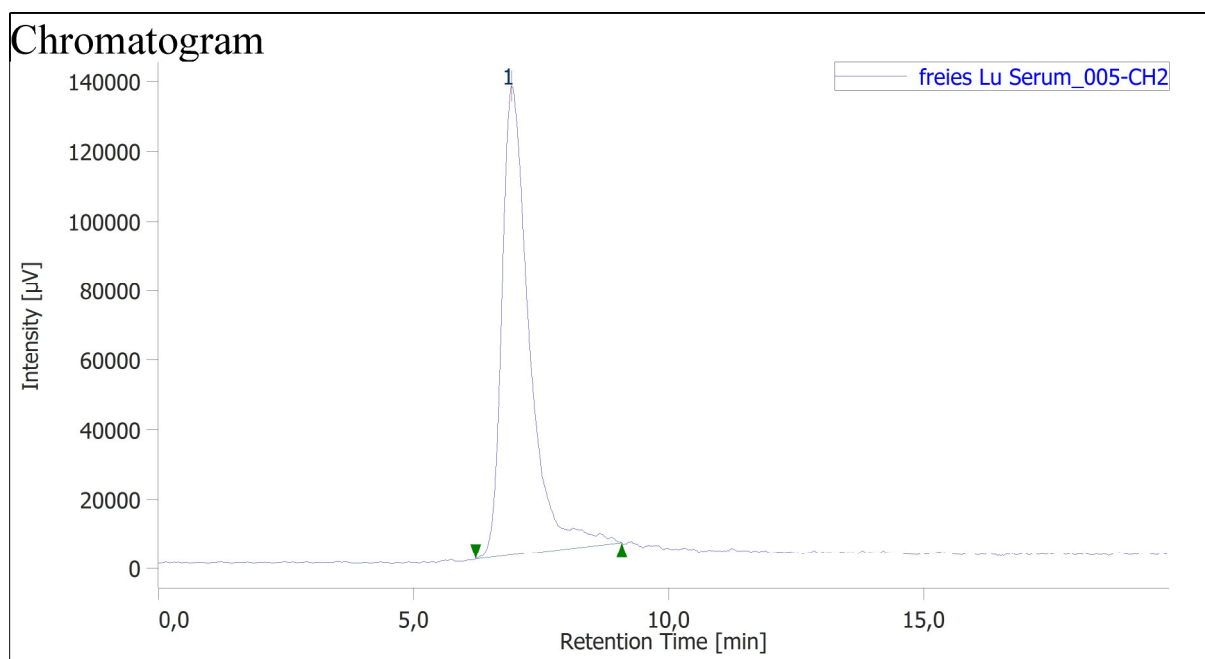

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,917	5029354	134649	100,000	100,000	954	N/A	1,632

