


Sample Name: Cu64-FK449

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Acq. Instrument : Agilent 1200                Location  :    4
Injection Date  : 7/7/2021 11:54:49 AM        Inj       :    1
                                           Inj Volume: 5.0 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 0.7 µl
Acq. Method     : C:\Chem32\1\Data\210707\Supersol 2021-07-07 10-40-38\SUPERSOL.M
Last changed    : 7/7/2021 10:40:38 AM by SYSTEM
Analysis Method : C:\Chem32\1\Methods\SUPERSOL.M
Last changed    : 6/15/2021 4:10:09 PM by SYSTEM
Additional Info  : Peak(s) manually integrated
=====

```

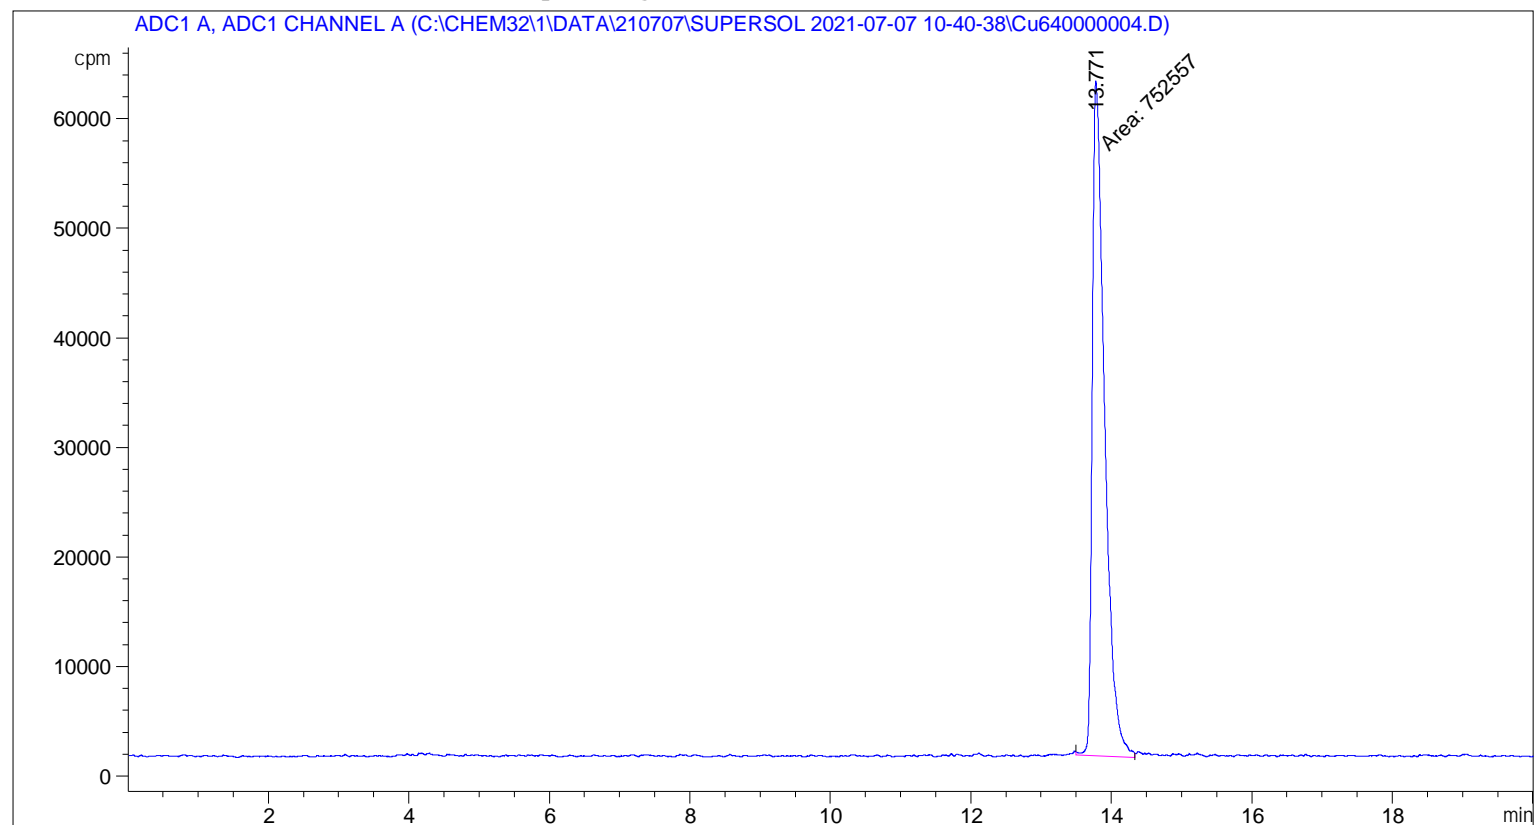

```

=====
                        Area Percent Report
=====

```

```

Sorted By           :      Signal
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: ADC1 A, ADC1 CHANNEL A

Peak #	RetTime [min]	Type	Width [min]	Area [cpm*s]	Height [cpm]	Area %
1	13.771	MM	0.2036	7.52557e5	6.15922e4	100.0000

```
Totals :                      7.52557e5  6.15922e4
```

```

=====
*** End of Report ***

```