


# Stabilitätstest

## Chromatogram Information

User Name user  
 Date Modified 08.09.2021 13:26:44  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 08.09.2021 13:06:54  
 Volume 10,00 [μL]  
 Sample # 4  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

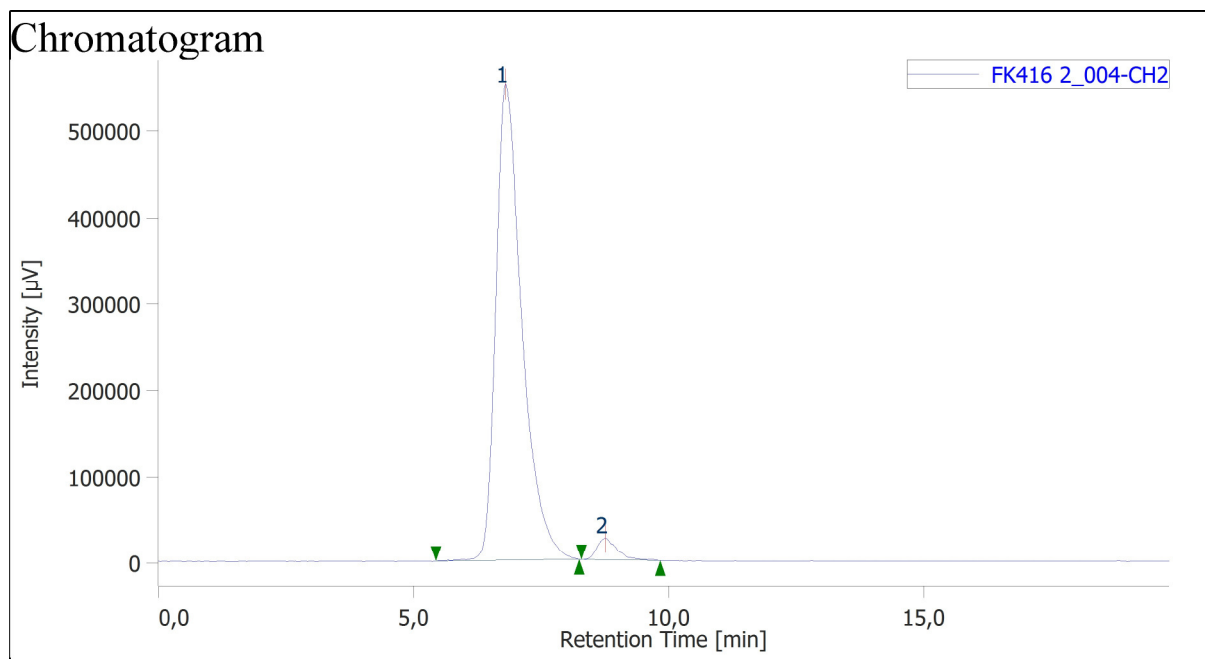

## Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,800	19589057	550366	96,468	95,468	936	2,470	1,580
2	Unknown	2	8,750	717162	26124	3,532	4,532	2540	N/A	1,604

