


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 25.03.2021 14:52:25
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 25.03.2021 11:44:29
 Volume 10,00 [μL]
 Sample # 4
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

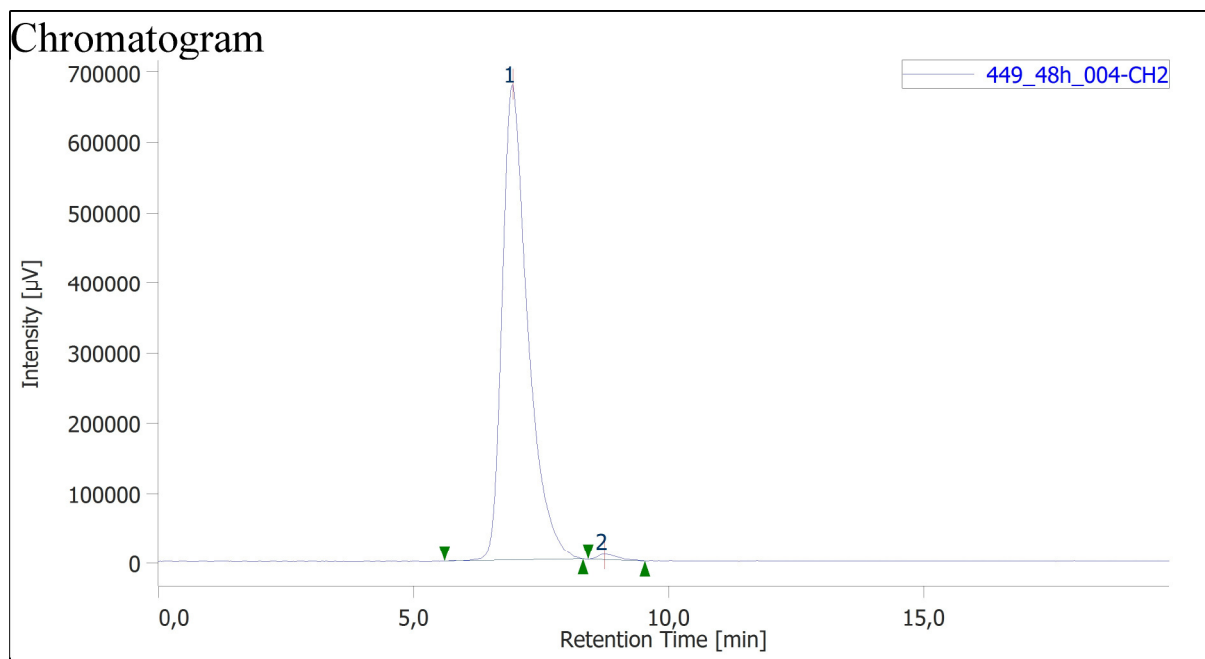

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	23551605	676820	99,063	98,833	1021	2,278	1,504
2	Unknown	2	8,742	222724	7989	0,937	1,167	2390	N/A	1,797

