


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 30.08.2021 16:34:07
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 30.08.2021 16:00:02
 Volume 30,00 [µL]
 Sample # 2
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

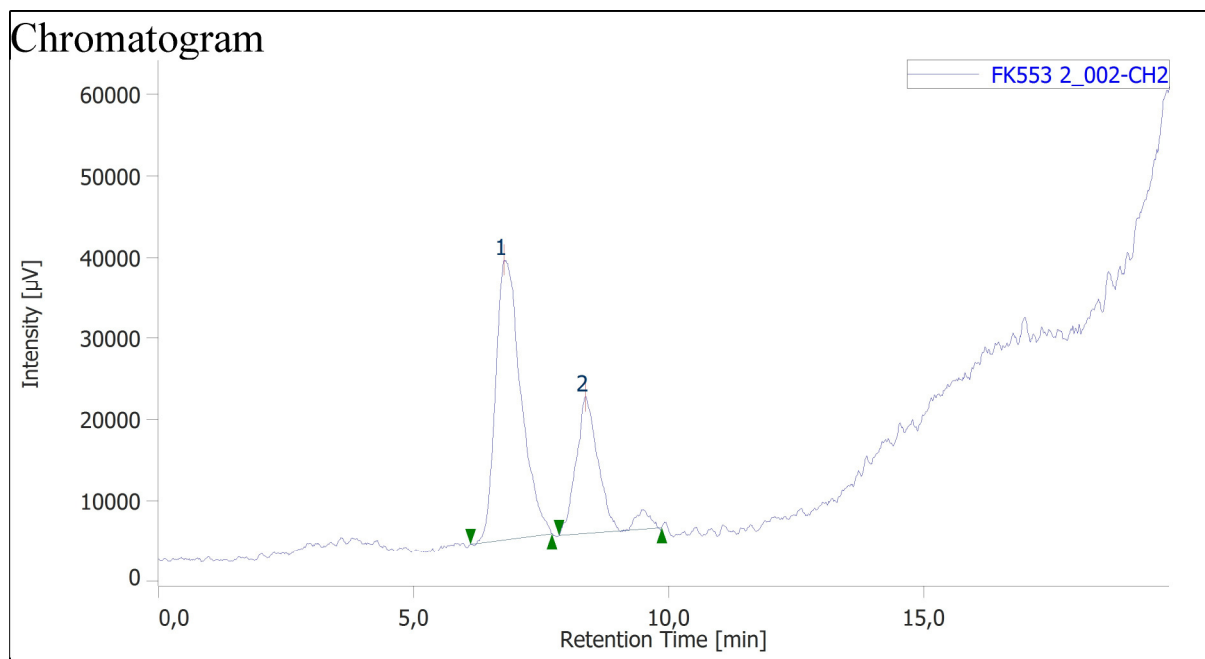

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,775	1184308	34536	68,689	67,230	945	1,904	1,547
2	Unknown	2	8,367	539847	16834	31,311	32,770	1772	N/A	1,907

