


## Stabilitätstest

### Chromatogram Information

User Name user  
 Date Modified 13.09.2021 12:32:19  
 Description  
 HPLC System Name Jasco-HPLC-1  
 Injection Date 13.09.2021 12:12:30  
 Volume 10,00 [µL]  
 Sample # 3  
 Project Name Lu-PDL1  
 Acquisition Time 19,8 [min]  
 Acquisition Sequence  
 Control Method PBS\_iso\_20min  
 Peak ID Table  
 Calibration Method  
 Additional Information  
 Column Info

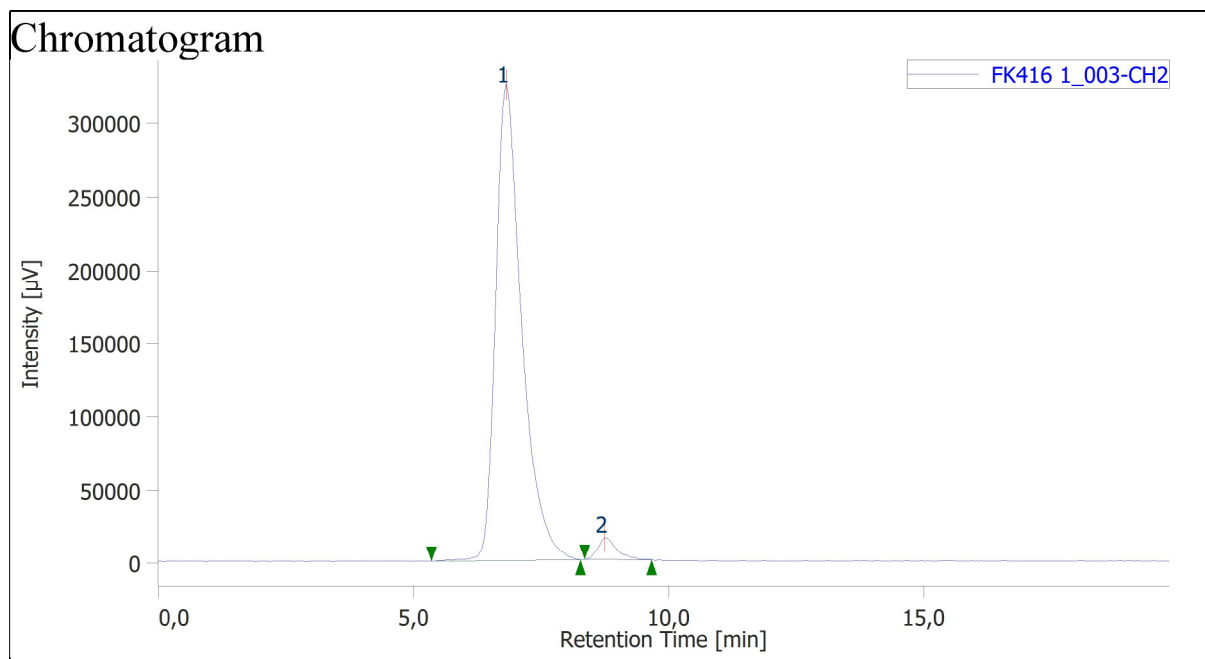

### Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,817	11520776	324136	96,662	95,438	953	2,544	1,497
2	Unknown	2	8,742	397816	15495	3,338	4,562	3041	N/A	1,491

