


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 30.03.2021 11:40:29
Description
HPLC System Name Jasco-HPLC-1
Injection Date 30.03.2021 10:03:06
Volume 10,00 [µL]
Sample # 3
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

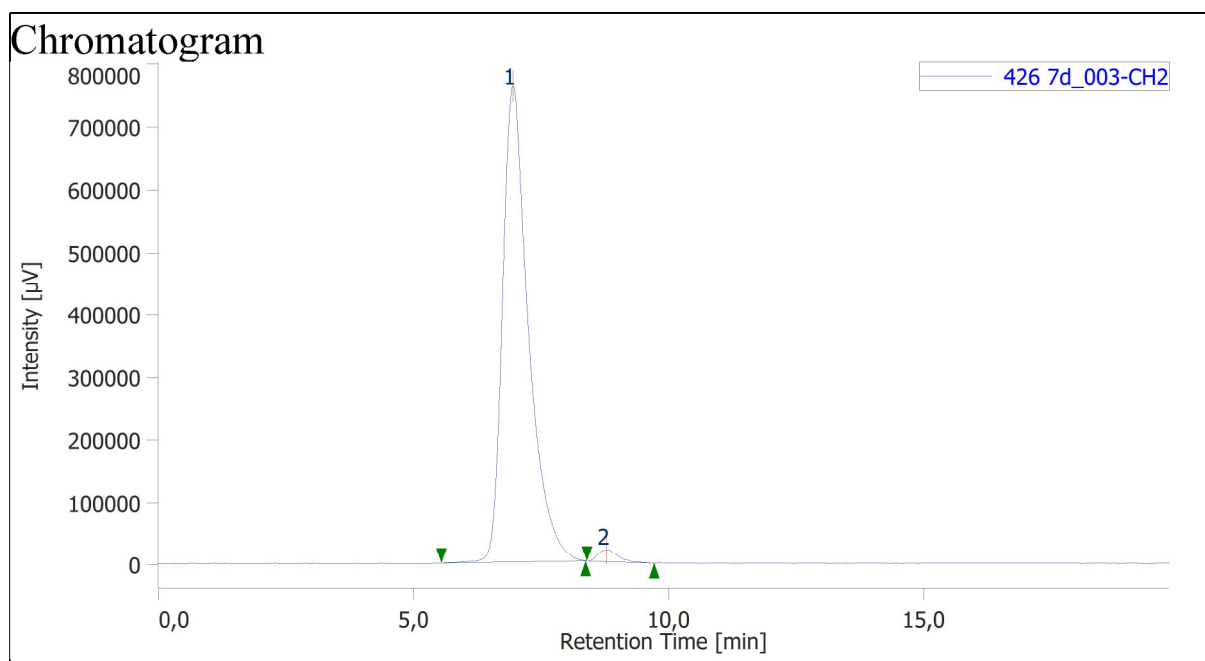

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	26899670	760299	98,073	97,443	1003	2,333	1,532
2	Unknown	2	8,783	528455	19954	1,927	2,557	2475	N/A	1,470

