


Stabilitätstest

Chromatogram Information

User Name user
 Date Modified 13.09.2021 15:21:06
 Description
 HPLC System Name Jasco-HPLC-1
 Injection Date 13.09.2021 15:03:17
 Volume 10,00 [μL]
 Sample # 1
 Project Name Lu-PDL1
 Acquisition Time 19,8 [min]
 Acquisition Sequence
 Control Method PBS_iso_20min
 Peak ID Table
 Calibration Method
 Additional Information
 Column Info

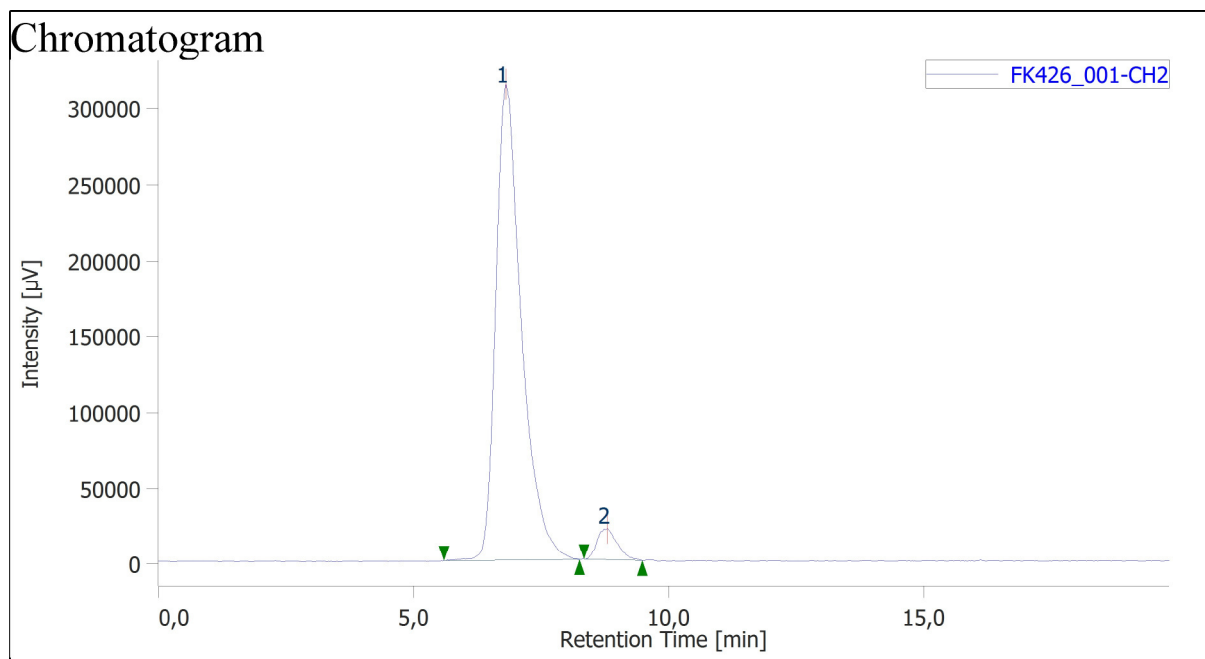

Peak Information

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,808	10929960	313071	95,050	93,749	980	2,460	1,504
2	Unknown	2	8,792	569250	20877	4,950	6,251	2218	N/A	1,242

