


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 30.03.2021 11:40:29
Description
HPLC System Name Jasco-HPLC-1
Injection Date 30.03.2021 10:45:16
Volume 10,00 [µL]
Sample # 4
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

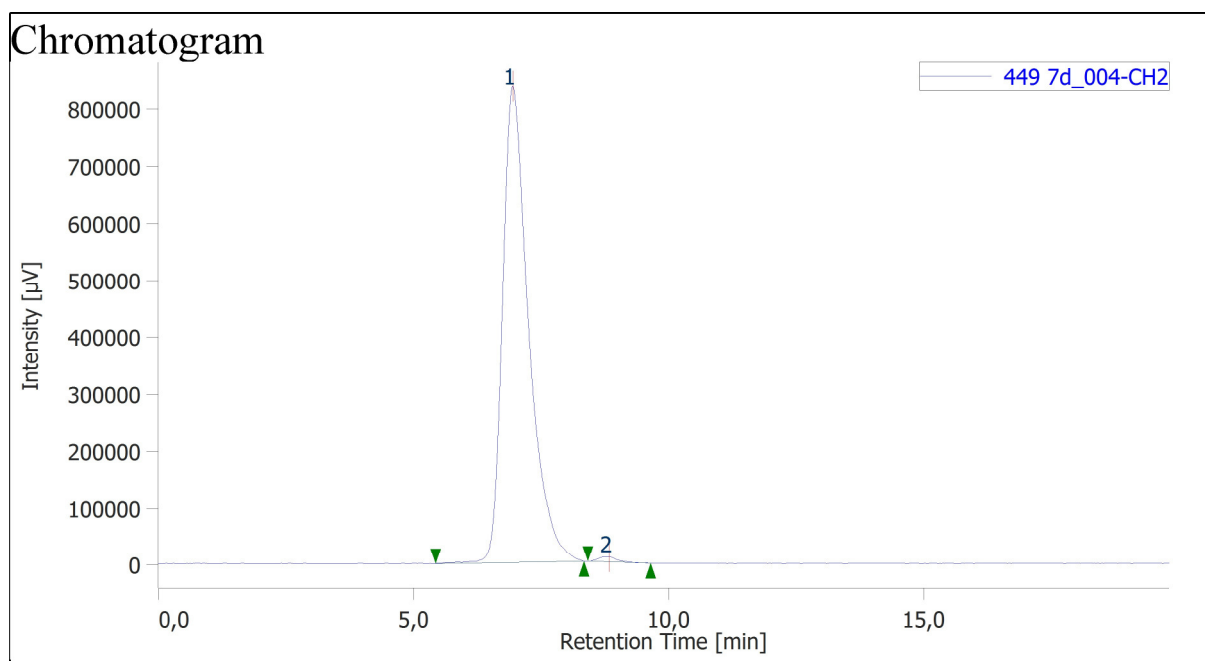

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,942	29732239	835237	99,230	98,935	982	2,491	1,519
2	Unknown	2	8,833	230565	8993	0,770	1,065	3079	N/A	1,075

