


Stabilitätstest

Chromatogram Information

User Name user
Date Modified 25.03.2021 14:52:25
Description
HPLC System Name Jasco-HPLC-1
Injection Date 25.03.2021 09:32:12
Volume 10,00 [µL]
Sample # 2
Project Name Lu-PDL1
Acquisition Time 19,8 [min]
Acquisition Sequence
Control Method PBS_iso_20min
Peak ID Table
Calibration Method
Additional Information
Column Info

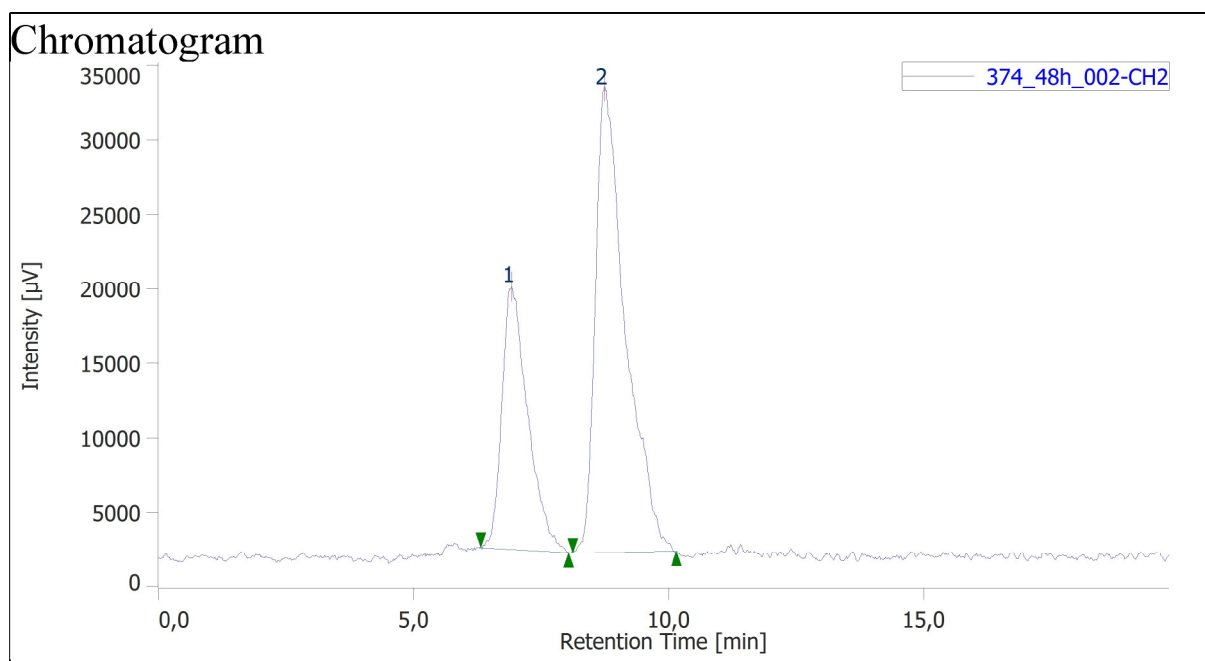

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	NTP	Resolution	Symmetry Factor
1	Unknown	2	6,925	621939	17643	32,774	36,064	890	1,915	1,536
2	Unknown	2	8,742	1275748	31278	67,226	63,936	1290	N/A	1,828

